



# BIOANALYSIS CATALOG



**GL Sciences Inc.**

**FROM SAMPLE PREPARATION TO  
ANALYTICAL SEPARATION**



Axel Kiers Vej 34 · 8270 Højbjerg · Denmark · CVR: DK 83309210  
Tel.: +45 8629 6111 · Fax: +45 8629 6122 · [mi@mikrolab.dk](mailto:mi@mikrolab.dk) · [www.mikrolab.dk](http://www.mikrolab.dk)

# Table of Contents

## Proteomics

---

Spin Column Trypsin Digestion.....	<b>MonoSpin Trypsin</b>
Market Leading Phosphopeptide Enrichment.....	<b>Titansphere 5 µm Bulk Media</b> <b>Titansphere 10 µm Bulk Media</b> <b>Titansphere Phos-TiO 10 µm Bulk Media</b> <b>NEW Titansphere Phos-TiO MP Kit</b> <b>Titansphere Phos-TiO Kit</b> <b>Titansphere Phos-TiO for Large Volume Sample</b>
Desalting Phosphopeptide-Enriched Samples.....	<b>GL-Tip SDB and GC</b>
Efficient Fractionation of Peptide Samples.....	<b>GL-Tip SCX and SDB-SCX</b>
Identification of Peptides/Proteins.....	<b>Meter Scale MonoCap HighResolution 2000 Series</b> <b>Other MonoCap Standard Length Columns</b>
Electrospray Emitter for ESI-LC/MS.....	<b>MonoSpray</b>

## Sample Preparation for LC/MS

---

Solid Phase Extraction Spin Columns.....	<b>MonoSpin and MonoSpin Large Type Series</b>
Protein Removal and Phospholipid Removal Plates.....	<b>FastRemover Series</b>
Desalting Phosphopeptide-Enriched Samples.....	<b>GL-Tip SDB and GC</b>
Efficient Fractionation of Peptide Samples.....	<b>GL-Tip SCX and SDB-SCX</b>

## Exosome

---

High Purity Exosome Isolation Columns.....	<b>EVSecond</b>
--	-----------------

## Antibody

---

Rapid Purification of Antibodies.....	<b>MonoSpin ProA and ProG</b>
---------------------------------------	-------------------------------

## DNA

---

Purification and Extraction of DNA.....	<b>MonoFas Series</b>
---	-----------------------

## Proteins

Spin Column Trypsin Digestion

### **MonoSpin Trypsin**



## Peptides

Market Leading Phosphopeptide Enrichment

**Titansphere 5 µm Bulk Media**

**Titansphere 10 µm Bulk Media**

**Titansphere Phos-TiO 10 µm Bulk Media**

**NEW Titansphere Phos-TiO MP Kit**

**Titansphere Phos-TiO Kit**

**Titansphere Phos-TiO for Large Volume Sample**



## Phosphopeptide

Desalting Phosphopeptide-Enriched Samples

### **GL-Tip SDB and GC**




Efficient Fractionation of Peptide Samples

### **GL-Tip SCX and SDB-SCX**

## LC/MS/MS

Identification of Peptides/Proteins

**Meter Scale MonoCap HighResolution 2000 Series**  
**Other MonoCap Standard Length Columns**

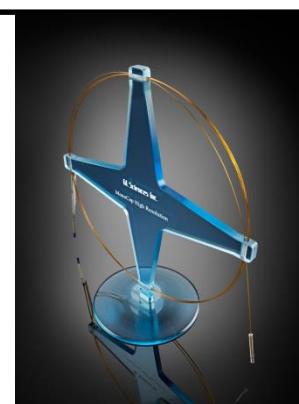

# Phosphorylation Purification & Enrichment

## Phosphorylated Protein Research

Protein phosphorylation is recognized as a fundamental process which regulates cell differentiation, growth, and migration. Analyzing protein phosphorylation is complicated by the low concentration of any given phosphoprotein and any one time, and the relatively low ionization efficiency of phosphopeptides in MS analysis. Therefore, enrichment of phosphopeptides and the relative reduction of non-phosphorylated peptides is critical to accurate analysis of protein digests by LC/MS.


GL Sciences' Titanium Dioxide (TiO<sub>2</sub> or Titania) products have emerged as the most effective means of phosphopeptide enrichment of protein digests prior to LC/MS analysis, replacing IMAC as the primary means of phosphopeptide sample pretreatment. Enrichment by titanium dioxide and IMAC, remain, however, complimentary techniques and are often used in combination to obtain optimal phosphopeptide analysis.

### What Makes GL Sciences' Titanium Dioxide Products Unique and Superior?

Titanium Dioxide exists in three crystalline forms, known as rutile, anatase, and brookite. Rutile and Anatase forms are the most common and most useful for phosphopeptide enrichment, and the ratio of rutile form to anatase form has significant implications for applicability to enrichment of phosphopeptides. GL Sciences' manufacturing technique for its phosphopeptide enrichment products produces a highly spherical bead with the optimum ratio of crystal forms of TiO<sub>2</sub>. The primary reason the GL Sciences' Pho-TiO products show superior performance is a direct result of the unique formulation of our titanium dioxide beads.

## Principal of Phosphopeptide Enrichment

### Adsorption Mechanism



Phosphate groups are preferentially adsorbed to the surface of titanium dioxide under acidic conditions and are eluted under basic conditions. Non-phosphorylated acid peptides non-specifically bound to the TiO<sub>2</sub> can be reduced by adding acid modifiers to the loading and/or wash buffers.

## Basics of Phosphopeptide Analyses by LC/MS/MS

Protein, Cell Tissues

SDS - PAGE

Gel Staining to ID Proteins

FPLC

Immunity Sedimentation

2D - PAGE

### Purification Enrichment of Phosphopeptide by GL Sciences' Titansphere TiO<sub>2</sub>

Reduction Alkylation  
Enzyme Digestion

Desalting

LC/MS/MS  
Analysis

## Titansphere™ Bulk Materials

### Bulk Sorbent Materials for Purification & Enrichment of Phosphopeptides


While GL Sciences' Phos-TiO spin columns based enrichment products are useful for most sample pretreatment applications, some investigators require bulk titanium dioxide media for specialized applications. Our market leading Titansphere Phos-TiO Kit is now available in bulk media which is Titansphere Phos-TiO 10  $\mu\text{m}$  bulk media, and is optimized for purifying and enriching more phosphopeptide.

## Applications

### Efficient Purification from HeLa Cell Lysate

The data at right shows the superior performance of Titansphere TiO using the HeLa Cell Lysate consisting mainly of non-phosphorylated peptides. Titansphere TiO shows exceptional selectivity - almost 90% of the bound peptides were phosphopeptides, and excellent capacity for total phosphopeptide binding. A competitive TiO product is shown, binding mainly non-phosphorylated peptides and a much lower total number of discreet phosphopeptide species.


Sample: HeLa Cell Lysate, Sample volume: 50  $\mu\text{g}$ ,  
Titansphere TiO volume: 1 mg

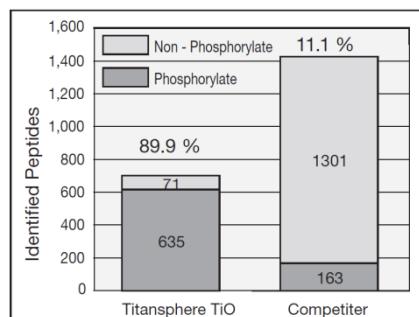

### Compare Titansphere TiO with IMAC

The graph at right shows how Titansphere TiO compares to an IMAC enrichment using Arabidopsis cell extract. Titansphere TiO provides substantially higher total capacity and a much higher number of discreet phosphopeptides isolated.

Sample: Arabidopsis Cell Extract, Sample volume: 100  $\mu\text{g}$ ,  
Titansphere TiO volume: 1 mg

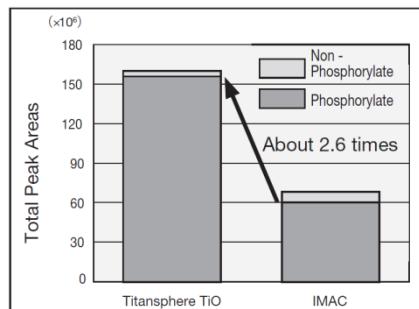

## Specifications

Description	Titansphere TiO
Particle Size	5 $\mu\text{m}$ , 10 $\mu\text{m}$
Particle Shape	Spherical
Adsorption Spot	Titanium Dioxide Crystal
Pore Size	100 $\text{\AA}$ (10 $\mu\text{m}$ )
pH Range	2 ~ 12
Gravity	1.74

## Ordering Information

### Titansphere™ Bulk Materials (Previous Version)

Description	Particle Size	Qty	Cat. No.
Titansphere TiO 5 $\mu\text{m}$ , 500 mg	5 $\mu\text{m}$	1/pk	5020-75000
Titansphere TiO 10 $\mu\text{m}$ , 500 mg	10 $\mu\text{m}$	1/pk	5020-75010

# **Titansphere™ Phos-TiO Bulk Material**

## **Titansphere™ Phos-TiO Bulk Material**

### **Bulk Sorbent Materials for Purification & Enrichment of Phosphopeptides**

---

While GL Sciences' Phos-TiO spin tips based enrichment products are useful for most sample pretreatment applications, some investigators require bulk titanium dioxide media for specialized applications. Our market leading Titansphere Phos-TiO Kit is now available in bulk media which is Titansphere Phos-TiO 10  $\mu$ m bulk media, and is optimized for purifying and enriching more phosphopeptide.

### **References**

---

1. Phosphopeptide enrichment by aliphatic hydroxy acid-modified metal oxide chromatography for nano-LC-MS/MS in proteomics applications, Sugiyama N, Masuda T, Shinoda K, Nakamura A, Tomita M, Ishihama Y., *Mol Cell Proteomics*. 2007 Jun;6(6):1103-9.
2. Highly selective enrichment of phosphorylated peptides using titanium dioxide, *Nature Protocols* 1, 2006, 1929-1935
3. Global, *in vivo*, and site-specific phosphorylation dynamics in signaling networks, Olsen JV, Blagoev B, Gnad F, Macek B, Kumar C, Mortensen P, Mann M., *Cell*. 2006 Nov 3;127(3):635-48.
4. Successive and selective release of phospholyated Peptides captured by Hydroxy Acid-Modified Metal Oxide Chromatography, Yutaka kyono, Naoyuki Sugiyama, Koshi Imami, Masaru Tomita, and Yasushi Ishihama, *J Proteome Res.*, 2008, 7(10), 4585-93
5. Extended coverage of singly and multiply phosphorylated peptides from a single Titanium Dioxide Microcolumn, *Anal Chem.*, 2015, 87(20), 10213-21

### **Ordering Information**

---

#### **Titansphere™ Phos-TiO Bulk Material (Same Bulk Media packed into Titansphere Phos-TiO Kit)**

<b>Description</b>	<b>Particle Size</b>	<b>Qty</b>	<b>Cat. No.</b>
Titansphere Phos-TiO Bulk 10um, 500 mg	10 $\mu$ m	1/pk	5010-21315

## NEW Titansphere™ Phos-TiO MP Kit

### Efficiently Enrich **BOTH** Singly and Multiply Phosphorylated Peptides

GL Sciences' is known as the best manufacturer for the enrichment/purification of phosphopeptide, which our Titansphere Phos-TiO kit and bulk resins are widely used throughout the world in major cancer research institutes and proteomics core facilities.

The new Titansphere Phos-TiO MP Kit employs a new protocol in the HAMMOC method, which enables highly efficient and selective recovery of not only singly, but also for multiply phosphorylated peptides. Specifically, the new kit fractions the singly and multiply phosphorylated peptides separately, which prevents ion suppression in LC-MS/MS detection and delivers higher recovery of multiply phosphorylated peptides.

### Features

- High Recovery of not only Singly, but also for Multiply Phosphorylated Peptides.
- All Operation is done using an Easy-To-Use Centrifuge.

### Sample Loading Capacity


Description	Content	
Sample	Tyr(PO <sub>3</sub> H <sub>2</sub> ) - Angiotensin II	
Spin Tip Sorbent Mass/Tip Volume	1 mg/ 200 µL	3 mg/200 µL
Sample Loading Capacity	1.2 µg	3.5 µg

### Titansphere Phos-TiO MP Kit Contents

Cat. No.	5010-21282	5010-21283
Titansphere Phos-TiO MP Kit	24 pcs	24 pcs
Titansphere Sorbent Mass/Tip Volume	1 mg / 200 µL	3 mg / 200 µL
Spin Tip Quantity	24 pcs (6 x 4 packs)	24 pcs (6 x 4 packs)
Waste Fluid Tube Quantity	24 pcs	24 pcs
Recovery Tube (2.0 mL) Quantity	24 pcs	48 pcs
Recovery Tube (1.5 mL) Quantity	48 pcs	48 pcs
Solution B (Lactic acid) Quantity	2 mL	2 mL
Instruction Manual	1/pk	1/pk

# NEW Titansphere™ Phos-TiO MP Kit

## Comparison of Recovery of **BOTH** Singly and Multiply Phosphorylated Peptides

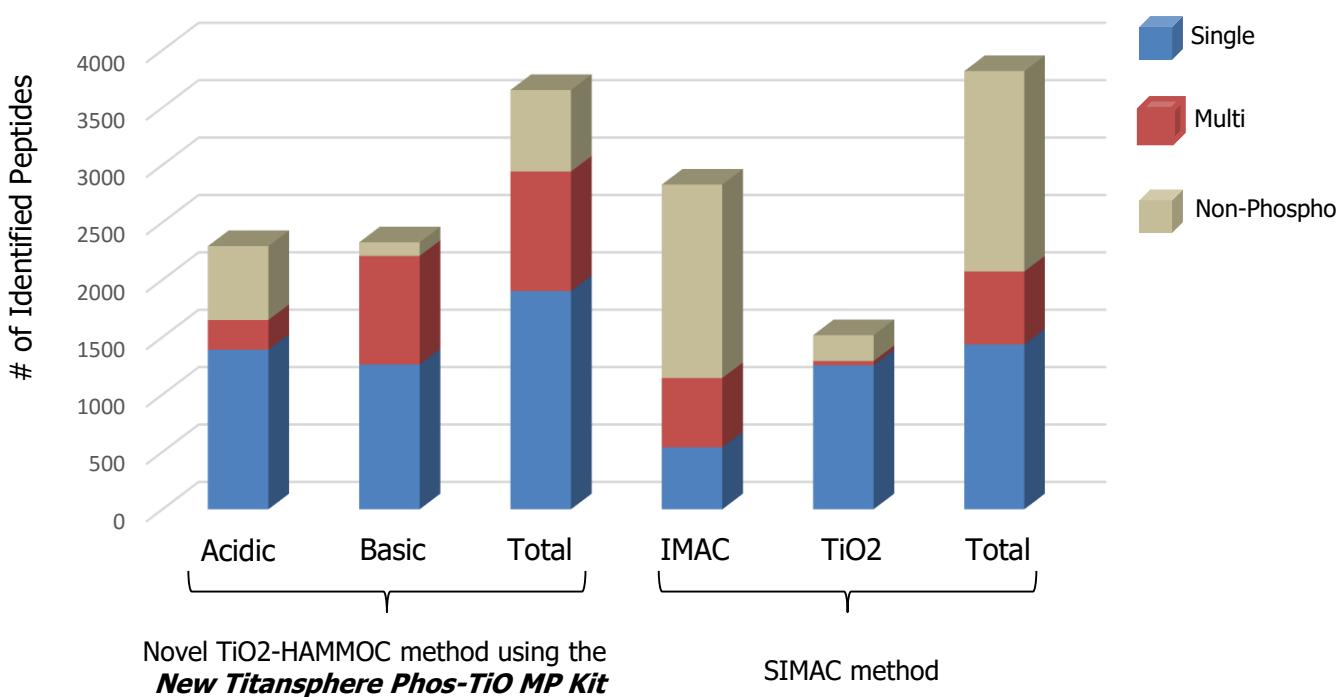

Novel TiO<sub>2</sub>-HAMMOC method using the  
**New Titansphere Phos-TiO MP Kit**

SIMAC method


Data from Wakabayashi et al. Ana Chem 2015, 87

The above experiment was done using HeLa cells 100 µg to prove the new Titansphere Phos-TiO MP Kit show highly efficient recovery of both singly and multiply phosphorylated peptides compared to SIMAC (Sequential Elution from IMAC) method.

The SIMAC method is generally separated into two major protocols, which the initial enrichment and separation of mono- and multi-phosphorylated peptides uses an Immobilized Metal ion Affinity Chromatography and a subsequent enrichment of the mono-phosphorylated peptides using titanium dioxide chromatography. Finally, the two separated phosphopeptide fractions are then analyzed by LC-MS/MS.

In the new Titansphere Phos-TiO MP Kit, singly phosphorylated peptides were recovered more when using an acidic elution buffer, while the multiply phosphorylated peptides were recovered more when using a basic elution buffer. As proven above, in total, the new Titansphere Phos-TiO MP Kit recovered more of both singly and multiply phosphorylated peptides than the SIMAC method.

## Typical Enrichment Protocol using Titansphere Phos-TiO MP Kit

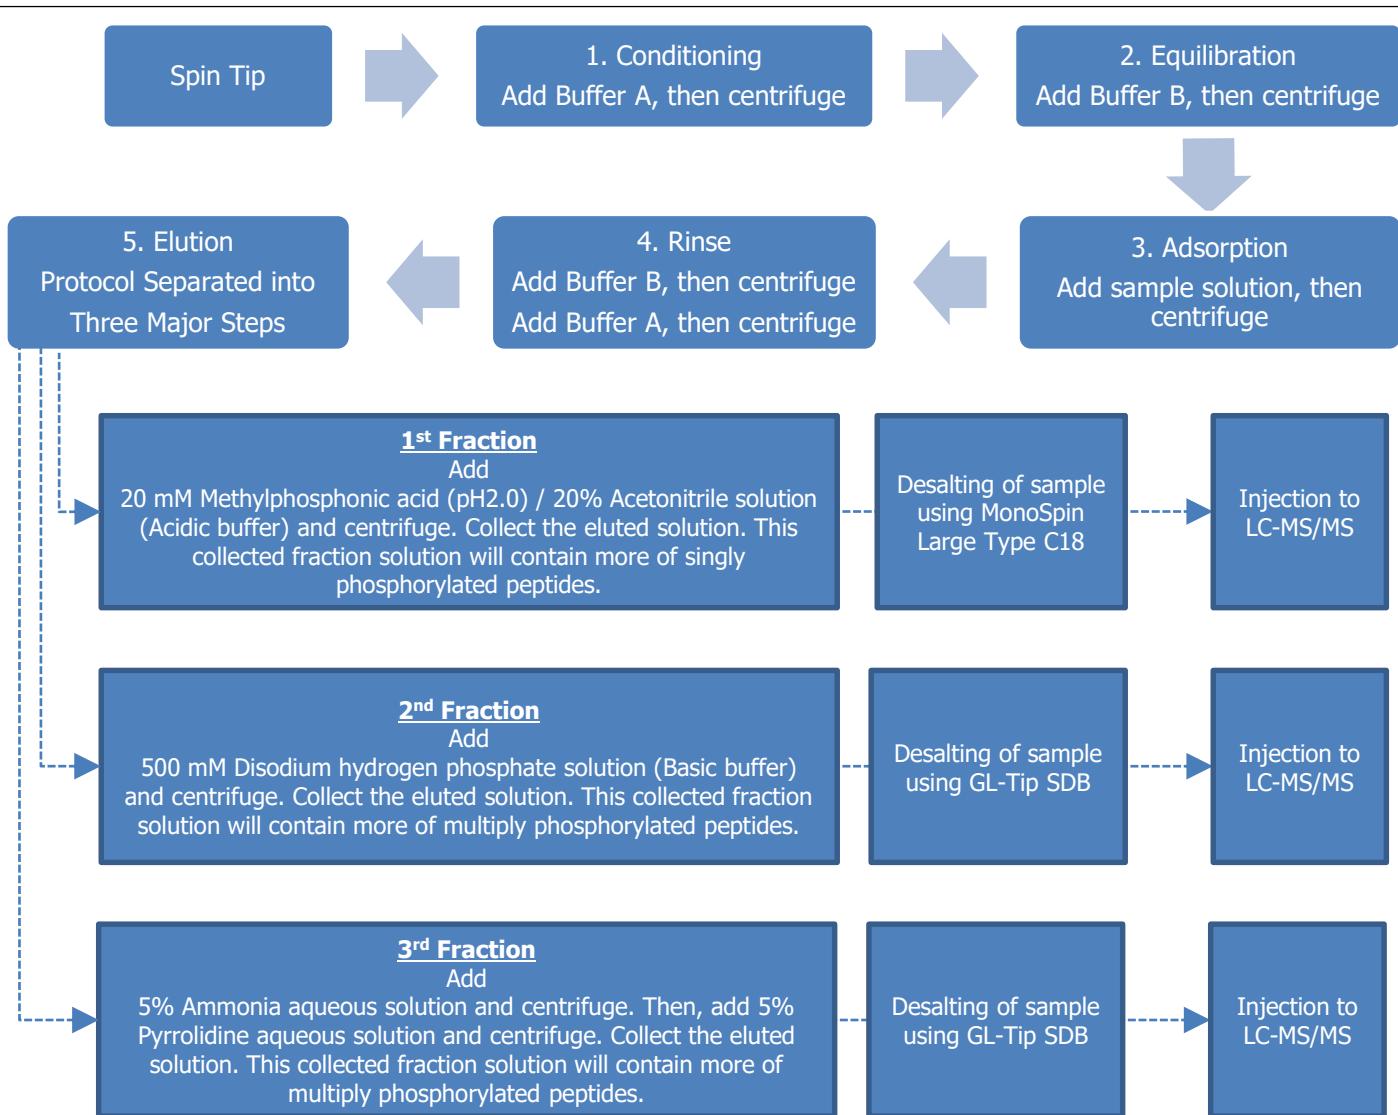**Remarks:**

- Buffer A, Buffer B, Methylphosphonic acid, Disodium hydrogen phosphate, Ammonia aqueous solution and 5% Pyrrolidine aqueous solution are not included in the kit due to their designation as hazardous materials for the purposes of air transportation. Therefore, the user must prepare these solutions in their lab, according to the procedure detailed in the instruction manual.
- Solution B is included in the kit, which is Lactic acid.
- The preparation procedure of Buffer A and B are as follows.

Buffer A	2% TFA solution	1mL
	Acetonitrile	4mL
	Total	5mL (Use 3mL for making Buffer B)

Buffer B	Solution B	1mL
	Buffer A	3mL
	Total	4mL

# NEW Titansphere™ Phos-TiO MP Kit

## Ordering Information

### Titansphere™ Phos-TiO MP Kit

- Centrifuge Adapter, 24 pcs/pk (Cat. No. 5010-21514) must be purchased once to use the Titansphere Phos-TiO MP Kit.
- This centrifuge adapter is reusable.
- Lactic acid is Solution B, which is already included in the kit, however, can be purchased separately for future requirements.

Description	Sorbent Mass/Tip Volume	Quantity	Cat. No.
Titansphere Phos-TiO MP Kit	1 mg / 200 mL	24 pcs	5010-21282
	3 mg / 200 mL	24 pcs	5010-21283
Centrifuge Adapter	-	24 pcs	5010-21514
Lactic acid for Titansphere Phos-TiO (This is Solution B included in the kit)	15 mL	1/pk	5010-21295

### Titansphere Phos-TiO MP Kit with Desalting Columns

- These special packages includes optimized desalting columns/spin tips to be used with Phos-TiO MP Kit.

Package Contents	Package Cat. No.
Titansphere Phos-TiO MP Kit, 1mg /200 mL, 24 pcs/pk (Cat. No. 5010-21282)	
MonoSpin Large type C18, 30 pcs/pk (Cat. No. 7510-11320)	5010-21272
GL-Tip SDB, 96 pcs/pk (Cat. No. 7820-11200)	

Package Contents	Package Cat. No.
Titansphere Phos-TiO MP Kit, 3mg /200 mL, 24 pcs/pk (Cat. No. 5010-21283)	
MonoSpin Large type C18, 30 pcs/pk (Cat. No. 7510-11320)	5010-21273
GL-Tip SDB, 96 pcs/pk (Cat. No. 7820-11200)	

### Titansphere Phos-TiO Spin Tips

- Spin tips are also available separately.

Description	Sorbent Mass/Tip Volume	Quantity	Cat. No.
	1 mg / 200 $\mu$ L	24 pcs	5010-21316
		96 pcs	5010-21317
Titansphere Phos-TiO Spin Tips	3 mg / 200 $\mu$ L	24 pcs	5010-21307
		96 pcs	5010-21308

## **Titansphere™ Phos-TiO Kit (Previous Version)**

### **Enrichment of Phosphopeptide Using Spin Tips**

This is the previous phosphopeptide enrichment kit that GL Sciences introduced to the market, which became the most popular kit worldwide. The titanium dioxide particles contained in the spin tips (available in 1 mg/10 µL and 3 mg/200 µL sizes) is specially treated to maximize selectivity for phosphorylated species, and the conditioning and washing buffers contain components to displace the few non-phosphorylated compounds which might originally adhere to the media.

### **Features**

- High Recovery of Singly Phosphorylated Peptides.
- All Operation is done using an Easy-To-Use Centrifuge.

### **Sample Loading Capacity**


<b>Description</b>	<b>Content</b>	
Sample	Tyr(PO <sub>3</sub> H <sub>2</sub> ) - Angiotensin II	
Spin Tip Sorbent Mass/Tip Volume	1 mg/ 10 µL	3 mg/200 µL
Sample Loading Capacity	1.2 µg	3.5 µg

### **Titansphere Phos-TiO Kit Contents**

<b>Cat. No.</b>	<b>5010-21309</b>	<b>5010-21310</b>	<b>5010-21311</b>	<b>5010-21312</b>
Titansphere Phos-TiO Kit for Export	24 pcs	96 pcs	24 pcs	96 pcs
Titansphere Sorbent mass/Tip Volume	1 mg / 10 µL		3 mg / 200 µL	
Spin Tip Quantity	24 pcs (6 x 4 packs)	96 pcs (6 x 16 packs)	24 pcs (6 x 4 packs)	96 pcs (6 x 16 packs)
Waste Fluid Tube Quantity	24 pcs	96 pcs	24 pcs	96 pcs
Recovery Tube Quantity	24 pcs	96 pcs	24 pcs	96 pcs
Solution B (Lactic acid) Quantity	2 mL	6 mL	2 mL	6 mL
Instruction Manual	1/pk	1/pk	1/pk	1/pk

# **Titansphere™ Phos-TiO Kit (Previous Version)**


## Phos-TiO Kits Outperform 4 Competitive TiO Based Products (MALDI-TOF/MS)

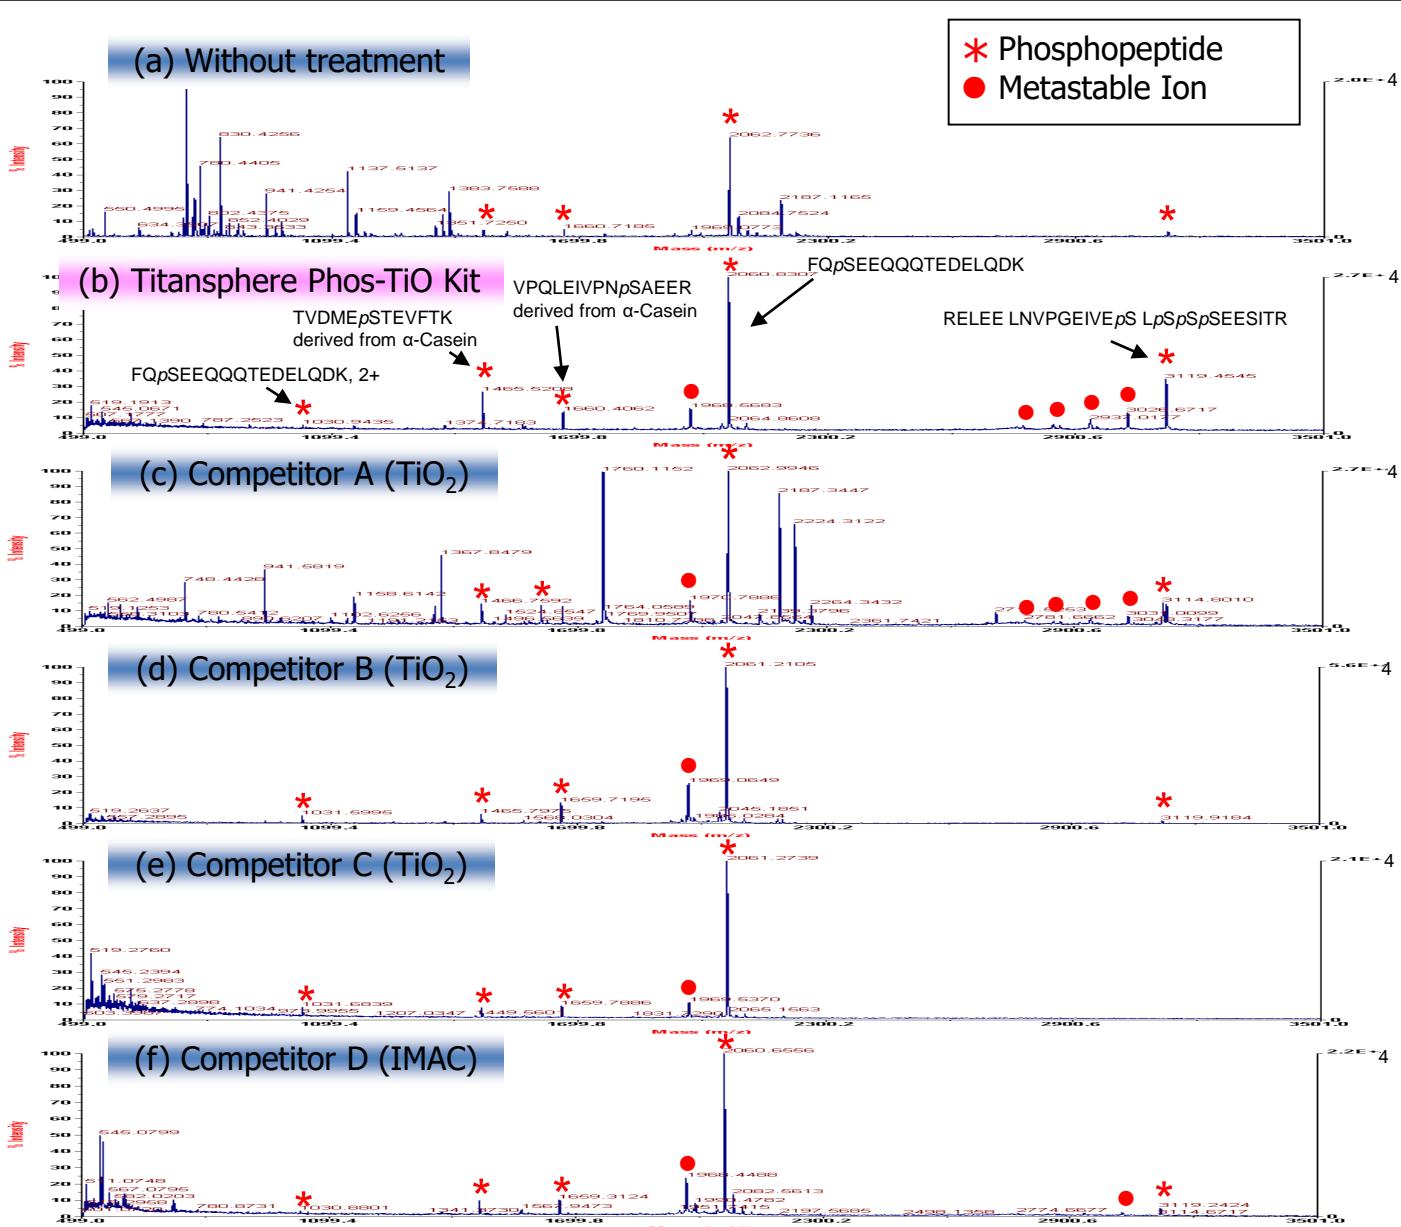

The data above show the purification efficiency of various TiO based products with a 2.5 µg sample of B-casein digest using MALDI-TOF/MS. Compared to the untreated condition (a), phosphopeptides were selectively purified when using Titansphere Phos-TiO Kit. Compared to competitive products (c to e) Titanpshere Phos-TiO Kit showed better selectivity. In general titanium dioxide is said that it has the worse adsorption efficiency of multi-phosphopeptides than IMAC. However, Titansphere Phos-TiO Kit showed higher selectivity, sensitivity and number of individual phosphopeptides isolated for 4 – phosphopeptides than IMAC (f). Metastable ion is a dephosphorylated peak.

## Comparison between GL Sciences' Previous Version Bulk Media

Optimal TiO beads (Titansphere Phos-TiO Bulk 10um, Cat No. 5010-21315) are used for Titansphere Phos-TiO Kit. The existing Titansphere TiO bulk media were improved for better adsorption capacity of phosphopeptides. Compared to the existing Titansphere bulk media (ex: Cat No. 5020-75000, 5020-75010), Phos-TiO Kit showed 2.6 times more peak area and 1.6 times more identified phosphopeptides.

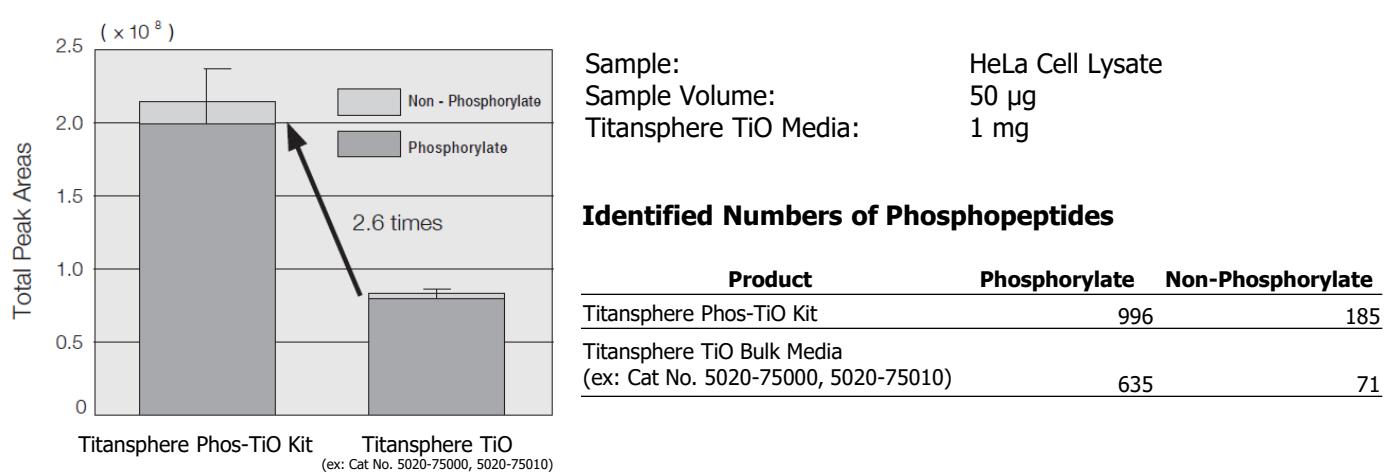

## Ordering Information

### Titansphere™ Phos-TiO Kit

- Centrifuge Adapter, 24 pcs/pk (Cat. No. 5010-21514) must be purchased once to use the Titansphere Phos-TiO Kit.
- This centrifuge adapter is reusable.
- Lactic acid is Solution B, which is already included in the kit, however, can be purchased separately for future requirements.

Description	Sorbent Mass/Tip Volume	Quantity	Cat. No.
Titansphere Phos-TiO Kit	1 mg / 10 µL	24 pcs 96 pcs	5010-21309 5010-21310
Titansphere Phos-TiO Kit	3 mg / 200 µL	24 pcs 96 pcs	5010-21311 5010-21312
Centrifuge Adapter	-	24 pcs	5010-21514
Lactic acid for Titansphere Phos-TiO (This is Solution B included in the kit)	15 mL	1/pk	5010-21295

### Titansphere Phos-TiO Spin Tips

- Spin tips are also available separately.

Description	Sorbent Mass/Tip Volume	Quantity	Cat. No.
	1 mg / 10 µL	24 pcs 96 pcs	5010-21302 5010-21303
Titansphere Phos-TiO Spin Tips	3 mg / 200 µL	24 pcs 96 pcs	5010-21307 5010-21308

# Titansphere™ Phos-TiO for Large Volume Samples

## Titansphere™ Phos-TiO for Large Volume Samples




### Appropriate for Larger Scale/Volume Purifications

The same specialized bulk media used in our Phos-TiO Kit is available in 50 mg/3 mL and 100 mg/3 mL cartridges as an extension of the Phos-TiO product line.

### Sample Loading Capacity

Description	Content	
Sample	Tyr(PO <sub>3</sub> H <sub>2</sub> ) - Angiotensin II	
Spin Tip Sorbent Mass/Tip Volume	50 mg/3 mL	100 mg/ 3 mL
Sample Loading Capacity	50 µg	100 µg

### Typical Enrichment Protocol using Titansphere Phos-TiO for Large Volume Samples

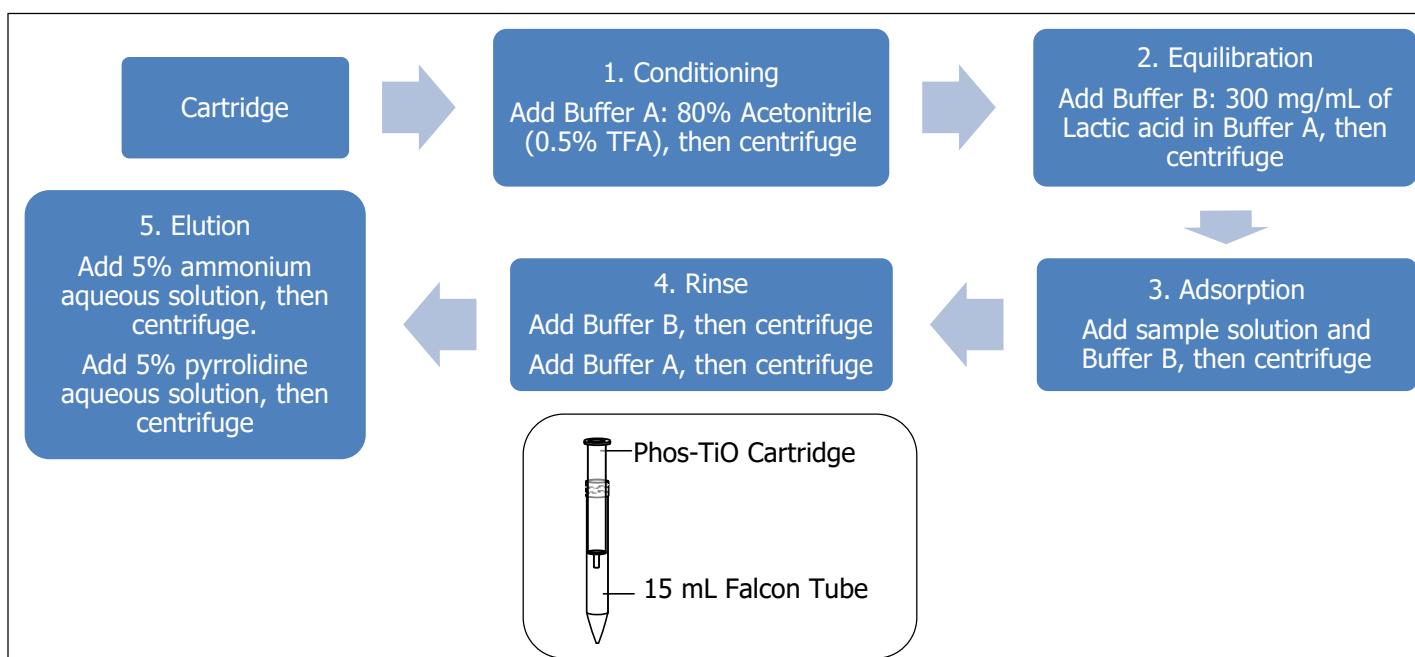

Phos-TiO for Large Volume Samples Cartridges are intended for use with a desktop or other centrifuge. While some of the versions of Phos-TiO are resemble pipette tips or SPE cartridges, these products are not intended for use with pipettes or SPE vacuum manifolds; the cartridge internal configuration and particle size of the TiO bulk media requires centrifugal elution of all solutions.

### Ordering Information

#### Titansphere™ Phos-TiO for Large Volume Samples

Description	Sorbent Mass/Tip Volume	Qty	Cat. No.
Titansphere Phos-TiO for Large Volume Samples	50 mg/3 mL	25 pcs	5010-21290
	100 mg/3 mL	25 pcs	5010-21291

## GL-Tip SDB and GL-Tip GC

### Desalting Phosphopeptide-Enriched Samples Prior to LC-MS/MS

Phosphopeptides isolated using TiO<sub>2</sub>-based medias are typically desalted prior to analysis by LC-MS/MS, typically using a C18 (hydrophobic) micropipette tip. GL Sciences' SDB (styrene divinylbenzene) and GC (graphite carbon) centrifuge-operated micropipette GL-Tip retain more hydrophobic and hydrophilic peptides, respectively, than C18-based tips.


### Features

GL-Tip SDB are more hydrophobic than C18 medias and allow retention of a wider range of phosphopeptides with high yield, allowing more accurate analysis of phosphopeptides species present in the sample. GL-Tip GC retain many more hydrophilic phosphopeptides than does C18; by using a combination of GL-Tip SDB and GC, almost all peptide samples can be desalted without sample losses due to lack of retention. Another highlight of this product is, the operation is very easy-to-use. Phosphopeptide-enriched samples are easily loaded, washed, and eluted using the same centrifuge-based technique used with Phos-TiO spin tips.

### Sample Loading Capacity

Description	GL-Tip SDB	GL-Tip GC
Sample	Tyr(PO <sub>3</sub> H <sub>2</sub> ) - Angiotensin II	Gly-Gly-Tyr-Arg
Spin Tip Sorbent Mass/Tip Volume	200 µL	1 mg/200 µL
Sample Loading Capacity	60 µg	30 µg



### Relative Retention of Peptides Collected using GL-Tip SDB and GC Desalting Tips

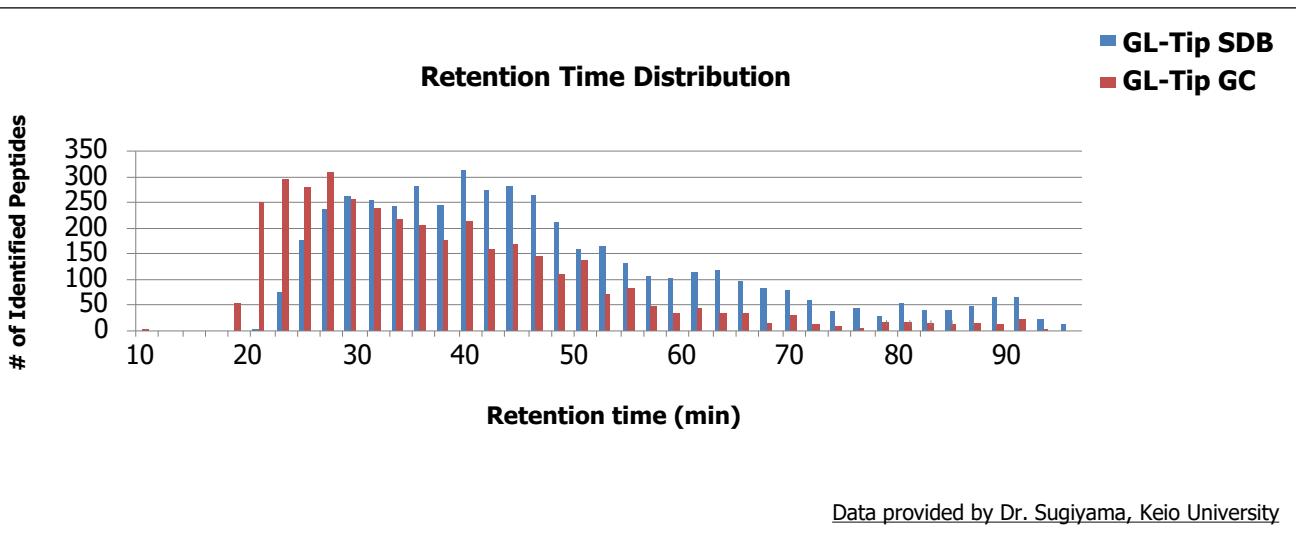

As illustrated above, the data indicating that GL-Tip SDB preferentially binds hydrophobic peptides while GC preferentially binds hydrophilic peptides.

# GL-Tip SDB and GL-Tip GC

## Recommended Protocol using GL-Tip SDB and GL-Tip GC

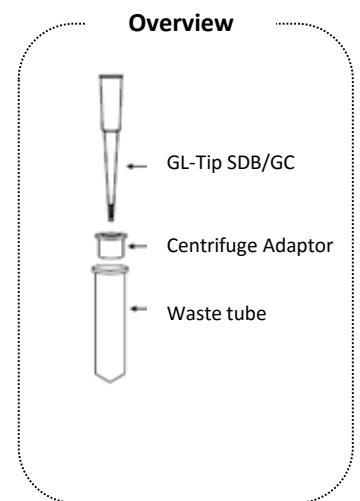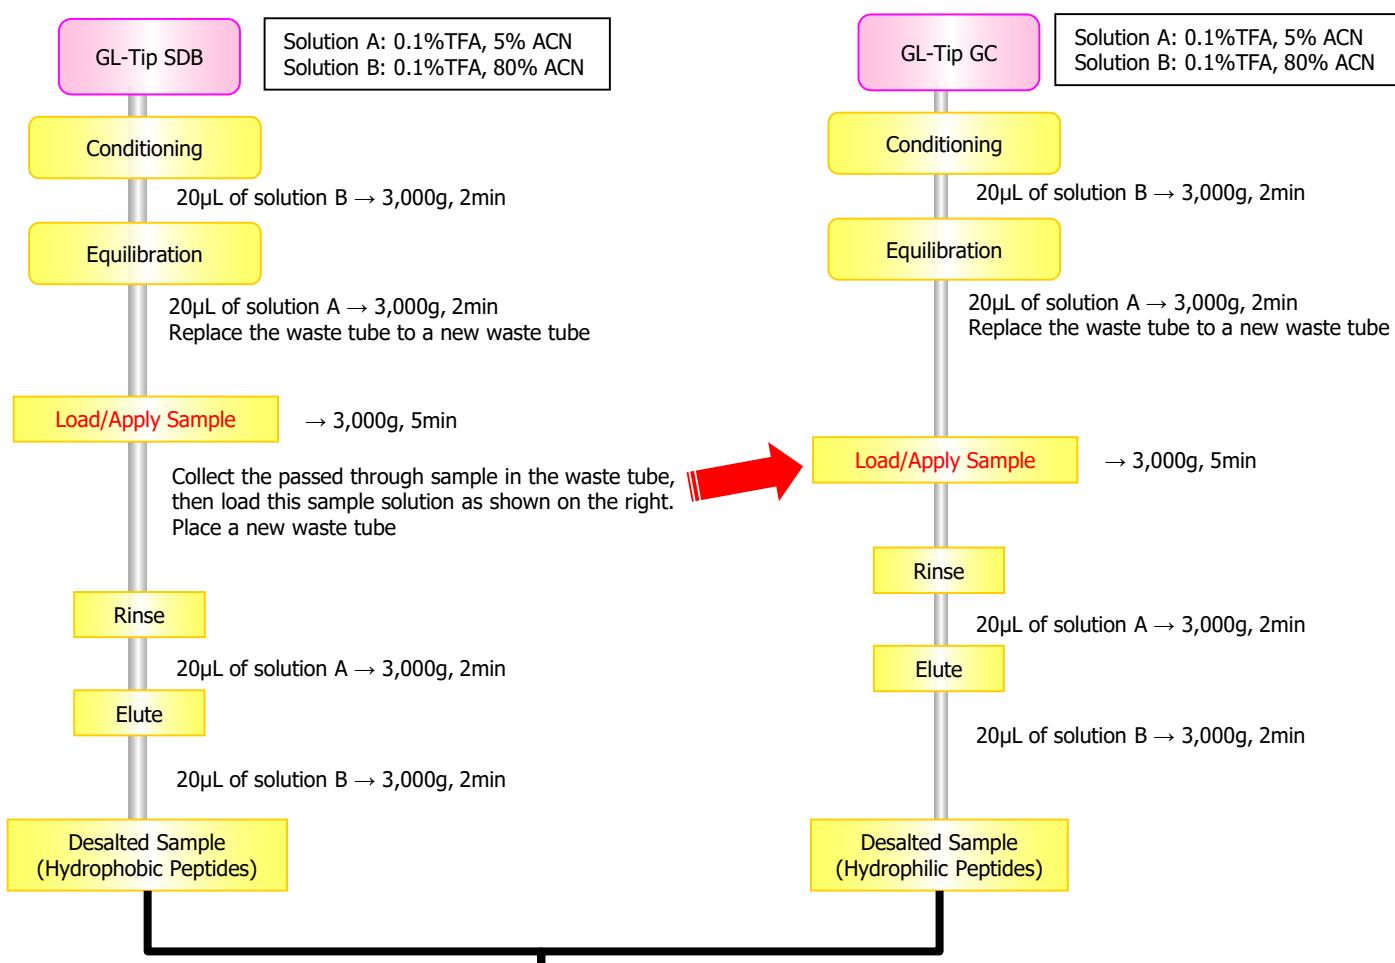


## Ordering Information

---

### GL-Tip SDB and GL-Tip GC

- Centrifuge Adapter, 24 pcs/pk (Cat. No. 5010-21514) must be purchased once to use the GL-Tip SDB and GL-Tip GC desalting spin tips.
- This centrifuge adapter is reusable.

Description	Tip Volume	Qty	Cat. No.
GL-Tip SDB	200 $\mu$ L	96 pcs	7820-11200
GL-Tip GC	200 $\mu$ L	96 pcs	7820-11201
Centrifuge Adapter	-	24 pcs	5010-21514

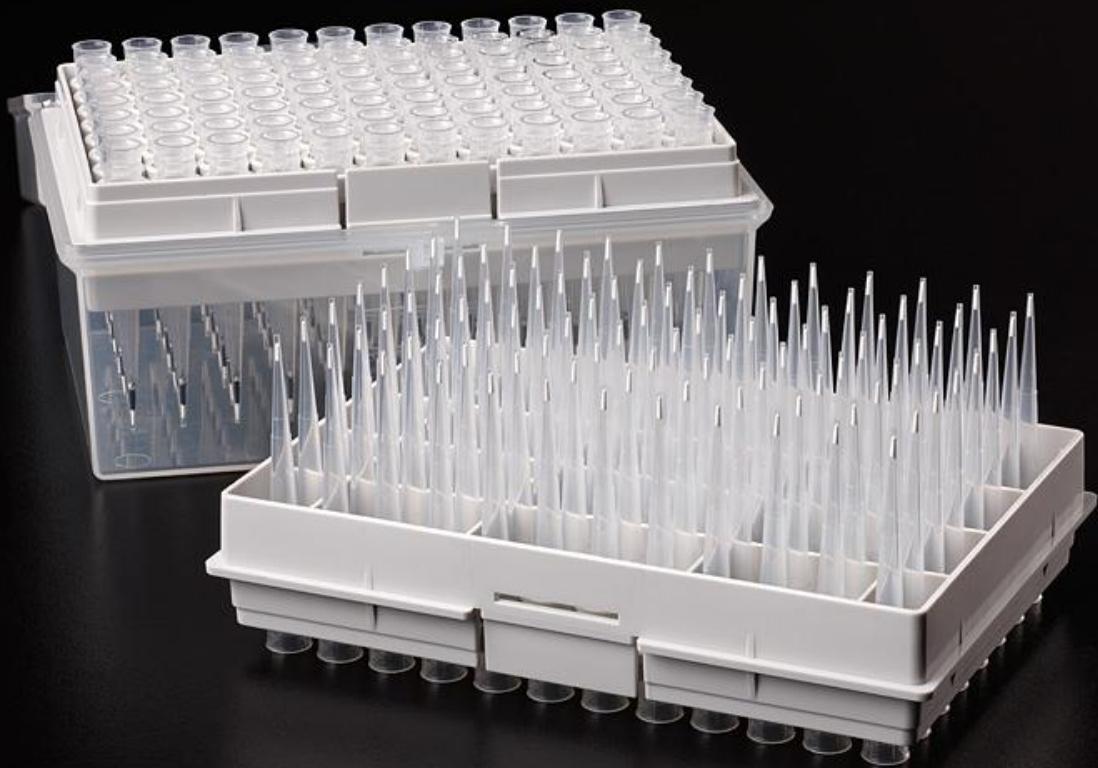

# GL-Tip SCX and GL-Tip SDB-SCX

## GL-Tip SCX and GL-Tip SDB-SCX

### Spin Tips for Peptide Fractionation

GL-Tip SCX is packed with strong cation polymer (SCX) and GL-Tip SDB-SCX are packed with styrene divinylbenzene polymer (SDB) and strong cation polymer (SCX). GL-Tip SDB-SCX is packed in a two layer format consisting an SDB and SCX media. Undesalted peptide samples can be used in GL-Tip SDB-SCX as the first SDB layer can desalt the sample.


### Sample Loading Capacity

Description	GL-Tip SCX	GL-Tip SDB-SCX
Sample	Angiotensin II	Angiotensin II
Tip Volume	200 $\mu$ L	200 $\mu$ L
Sample Loading Capacity	60 $\mu$ g	60 $\mu$ g


### Comparison of Traditional Gradient Elution vs TFA Gradient Elution

#### Comparison of Efficiency between Traditional Gradient Elution vs TFA Gradient Elution using DLD-1 Human Large Intestinal Cancer Cell derived Phosphopeptides

<NEW TFA Gradient Elution using GL-Tip SDB-SCX>

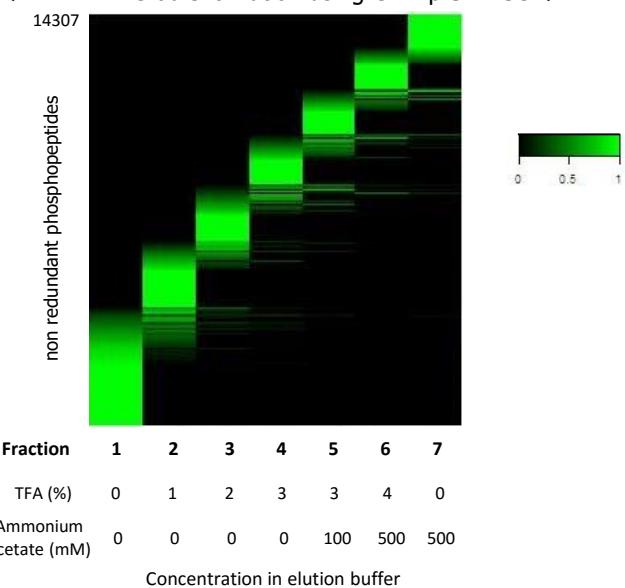

<Traditional Gradient Elution using GL-Tip SDB-SCX >

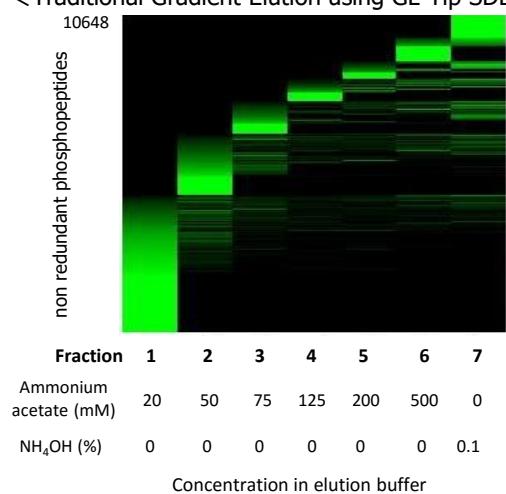


As proven above, the newly developed TFA gradient elution identified 14307 peptides promising higher efficiency than the traditional gradient elution method.

(Data provided from the National Institute of Biomedical Innovation, Dr. Jun Adachi)

A gradient elution using cation SCX media is commonly used in shotgun proteomics to fractionate peptide samples from complex samples such as cell or tissue extracts. The biggest challenge arises when identifying the same peptide from one fractionated peptide sample to another, which results in lowering efficiency. The newly developed TFA gradient elution method (patent applied) identifies more peptides without decreasing operation efficiency.

## Comparison of Number of Quantified Peptides

Compared results between commercially available brand G's tip column. GL-Tip SCX recovered more peptides. The usage of the newly developed TFA gradient elution method provide less chance of identifying the same peptide from one fractionated sample peptide to another resulting in higher efficiency.

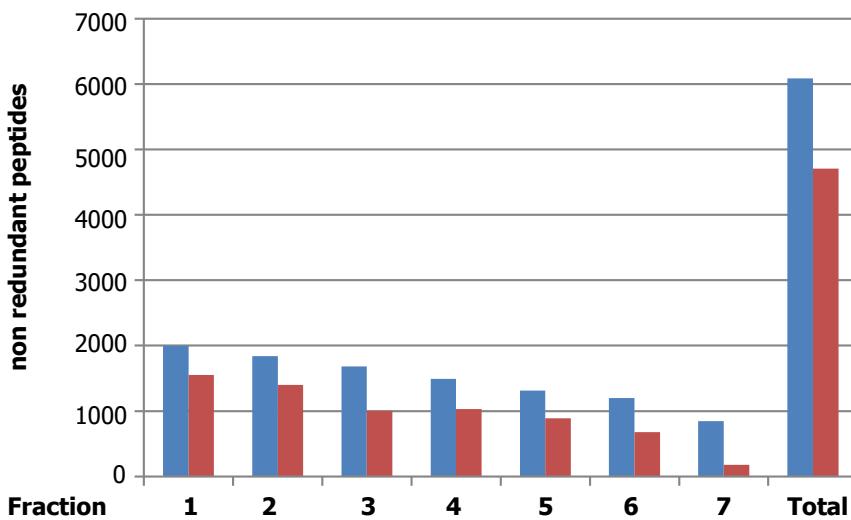

GL-Tip SCX

Brand G

### Sample/Procedure:

Trypsin digestion of HeLa cell lysate 25 µg each were fractionated and 40% of the recovered sample were identified via LTQ-Orbitrap XL, 45 minutes gradient using Maxquant 1.5.1.2, uniprot human database.

### Number of Identified Non Redundant Peptides

Fractions	1	2	3	4	5	6	7	total
GL-Tip SCX	1996	1839	1684	1491	1311	1196	847	6085
Brand G	1552	1397	1004	1032	890	676	179	4704

(Data provided from the National Institute of Biomedical Innovation, Dr. Jun Adachi)

## Ordering Information

### GL-Tip SCX and GL-Tip SDB-SCX


- Centrifuge Adapter, 24 pcs/pk (Cat. No. 5010-21514) must be purchased once to use the GL-Tip SCX and GL-Tip SDB-SCX peptide fractionation spin tips.
- This centrifuge adapter is reusable.

Description	Tip Volume	Qty	Cat. No.
GL-Tip SCX	200 µL	96 pcs	7510-11203
GL-Tip SDB-SCX	200 µL	96 pcs	7510-11202
Centrifuge Adapter	-	24 pcs	5010-21514
Centrifuge Adapter for 96-Well Plate	-	1/pk	5010-21341
Centrifuge Adapter for 96-Well Plate	-	2 pcs	5010-21343



## MonoCap HighResolution 2000 Series

Optimized for Identification of Peptides/Proteins for Proteome Research

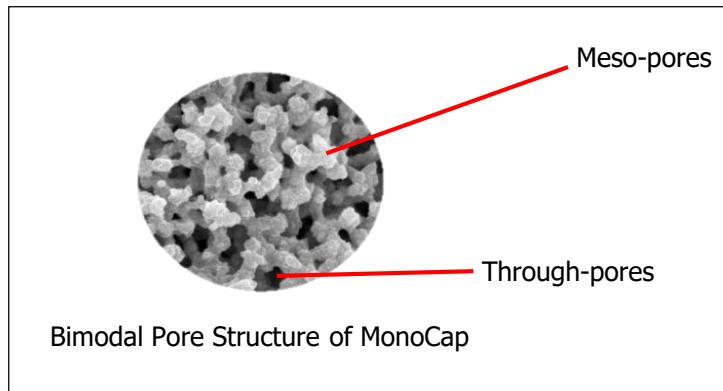

MonoCap HighResolution 2000 is a 2 meter length monolithic silica capillary column which is designed for identifying extremely high number of peptides/proteins for proteome research via LC-MS/MS.

GL Sciences' MonoCap capillary columns, created synthetically via sol-gel method, and an octadecyl silane chemically bonded, has a very uniform three dimensional structure that shows excellent reproducibility from batch-to-batch. The solid structure of GL Sciences' monolithic silica eliminates the need for frits or filters at the ends of the column, thereby reducing dead volume that might otherwise lead to band broadening or sample recovery. The high porosity of our monolithic silica allows high flow rates to be used without loss of resolution or creation of high operating pressure. An optimized balance of through-pores and meso-pores provides the critically important combination of efficiency, separation speed, large volume sample-loading, and small volume sample-recovery.

MonoCap HighResolution provide extremely high efficiency, delivering over 200,000 plates for a 2,000 mm length column. The MonoCap HighResolution Ultra type deliver over 300,000 plates.

### Physical Properties

Product Description	Bonded Phase	Meso-pore	End-capping	Max. Operating Pressure
MonoCap C18 HighResolution 2000	Octadecyl Groups	15 nm	Yes	35 MPa
MonoCap C18 HighResolution Ultra 2000	Octadecyl Groups	11 nm	Yes	35 MPa
MonoCap HILIC-UP HighResolution 2000	Ureidopropyl Groups	12 nm	None	35 MPa

Based on monolithic technology, Merck KGaA, Darmstadt, Germany.




## Discover New Peptides/Proteins

As proven below, MonoCap C18 HighResolution 2000 mm length column identifies simply more peptides/proteins compared to those traditional particle packed capillary HPLC columns.


MS: LTQ-Orbitrap XL (Mascot Search)  
 Sample: THP-1 Cell Lysate Tryptic Digest, 5  $\mu$ g

Column Name	Number of Identified Proteins in average	Analysis Time
<b>MonoCap C18 HighResolution 2000 0.1 mm I.D. x 2000 mm</b>	<b>2,087 (2013, 2116, 2131)</b>	<b>10 Hours</b>
Particle packed column 0.1 mm I.D. x 150 mm	680 (685, 679, 675)	2 Hours

**[1] MonoCap C18 HighResolution 2000 (2000 mm x 0.1 mm I.D.)**

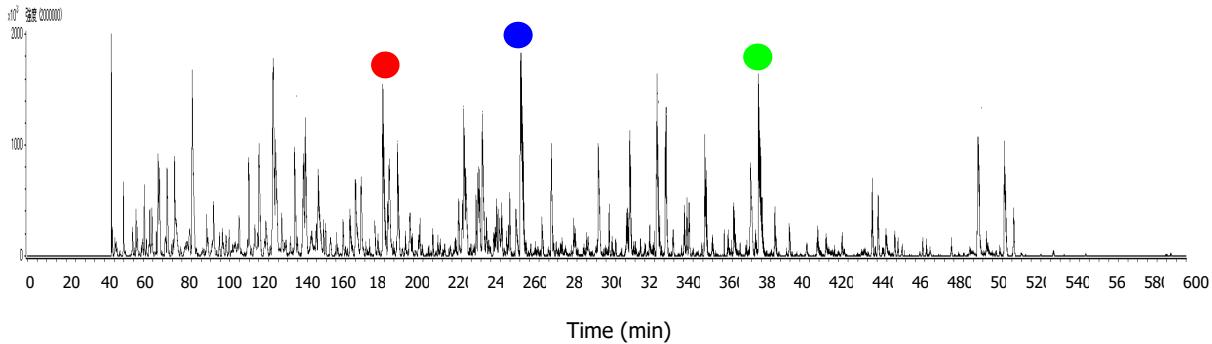

**[2] Particle Packed column (3  $\mu$ m , 150 mm x 0.075 mm I.D.)**

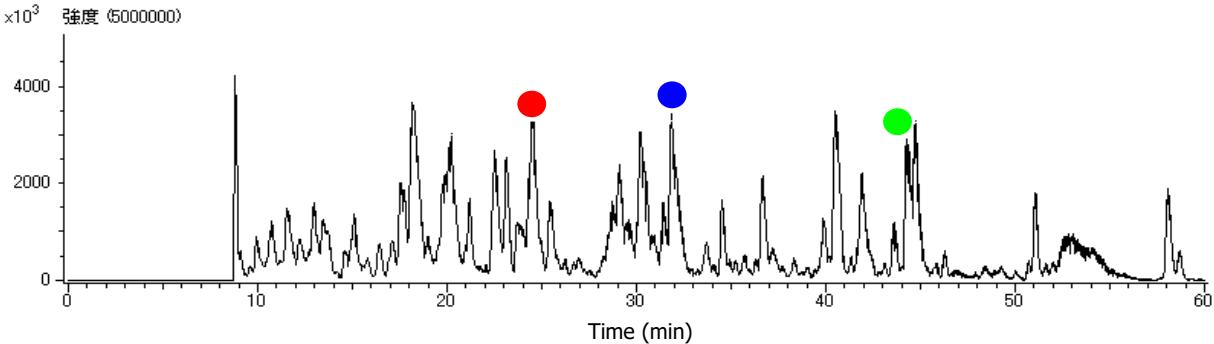

**Conditions**

System	: GLS Capillary HPLC system	Flow Rate	: [1] 0.5 $\mu$ L/min [2] 0.3 $\mu$ L/min
Column	: [1] MonoCap C18 High Resolution 2000 (2000 mm x 0.1 mm I.D.)	Injection Vol.	: 5 $\mu$ L
Trap column	: [2] Particle packed column (3 $\mu$ m, 150 mm x 0.075 mm I.D.)	Detection	: MS (TIC m / z 500-1500)
Eluent	: MonoCap C18 Trap Column (50 mm x 0.075 mm I.D.) : A) 0.1 %HCOOH in $\text{CH}_3\text{CN}$ : B) 0.1 %HCOOH in $\text{H}_2\text{O}$ [1] A / B = 10 / 90 - 600 min - 45 / 55 [2] A / B = 10 / 90 - 180 min - 45 / 55	Sample	: Tryptic digest of proteins


● ● ● are analytes having the same molecular weight

# MonoCap HighResolution 2000 Series


## For Identifying Highly Hydrophilic, Hydrophobic Peptides/Proteins

MonoCap HILIC-UP is an important addition to the MonoCap C18 HighResolution 2000 column series. MonoCap HILIC-UP can retain highly hydrophilic peptides/proteins which may lead to discovering new peptides/proteins where a C18 phase couldn't identify.

In HILIC, the higher the organic concentration, the greater the retention of more polar analytes. One of the biggest benefit of HILIC mode is, a high organic solvent concentration of the mobile phase will lead to a high sensitivity LC-MS/MS analysis.

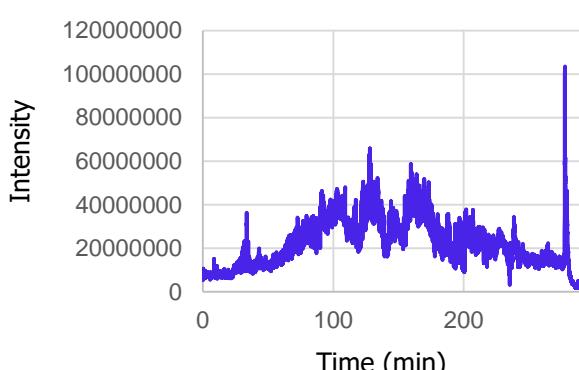

Total Ion Chromatogram

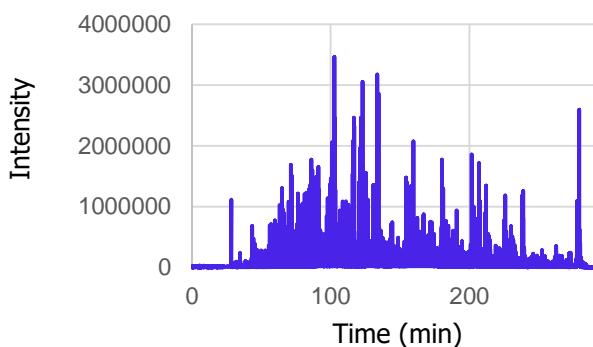

Base Peak Chromatogram

### Remarks:

#### Results of MonoCap C18 HighResolution 2000

Number of Identified Peptides: 8,358

Number of Identified Proteins: 1,992

Gradient Program: 4 hrs

#### Results of MonoCap HILIC-UP HighResolution 2000

Number of Identified Peptides: 7,194 (14,736 PSM\*)

Number of Identified Proteins: 2,201

\* Peptide Spectrum Match

### Conditions

Column	: MonoCap HILIC-UP High Resolution 2000
Eluent	: A) CH <sub>3</sub> CN : H <sub>2</sub> O=10/90 (0.5% CH <sub>3</sub> COOH) B) CH <sub>3</sub> CN : H <sub>2</sub> O=95/5 (0.5% CH <sub>3</sub> COOH) A/B=0/100-(240 min)-20/80-(10 min)-100/0-(10 min)-100/0
Flow Rate	: 0.5 μL
Injection Vol.	: 1 μL (1 mg/mL)
Detection	: TIC MS (m/z 300-1500)
Sample	: Tryptic Digest of Hela Cell Lysate, 5 ug

### Reference:

Hydrophilic Interaction Chromatography Using a Meter-Scale Monolithic silica capillary Column for Proteomics LC-MS,  
K Horie et al. *Anal. Chem.* 2014, 86, 3817-3824

## References

---

1. M.H.M. van de Meent et al.  
Improvement of the liquid-chromatographic analysis of protein tryptic digests by the use of long-capillary monolithic columns with UV and MS detection, *Anal Bioanal Chem*, 2007, 388, 195-200
2. Mio Iwasaki et al.  
One-Dimensional Capillary Liquid Chromatographic Separation Coupled with Tandem Mass Spectrometry Unveils the *Escherichia coli* Proteome on a Microarray Scale, *Anal. Chem.* 2010, 82, 2616-2620
3. Mio Iwasaki et al.  
Human Proteome analysis by using reversed phase monolithic silica capillary columns with enhanced sensitivity, *J Chromatogr A* 2012, 1228, 292-297
4. Ryota Yamana et al.  
Rapid and deep profiling of human induced pluripotent stem cell proteome by one-shot NanoLC-MS/MS analysis with meter-scale monolithic silica columns, *J Proteome Res.* 2013, 12, 214-21
5. Mari Ogawa-Ohnishi et al.  
Identification of three hydroxyproline O-arabinosyltransferases in *Arabidopsis thaliana*, *Nature Chem. Biol.* 2013, 9, 726-730
6. Satoru Okamoto et al.  
Root-derived CLE glycopeptides control nodulation by direct binding to HAR1 receptor kinase, *Nature Commun.* 2013, 4, 2191
7. Kanta Horie et al.  
Hydrophilic interaction chromatography using a meter-scale monolithic silica capillary column for proteomics LC-MS, *Anal. Chem.* 2014, 86, 3817-3824

# MonoCap HighResolution 2000 Series

## Ordering Information

### MonoCap C18 HighResolution Ultra 2000

- End-fittings are not included.
- A column connection kit is available separately to ensure proper connections.
- Please refer to the below ordering information.

Description	I.D. (mm)	Length (mm)	Qty	Cat. No.
MonoCap C18 HighResolution Ultra 2000	10 $\mu\text{m}$	2000	1/pk	5020-10018

### MonoCap C18 HighResolution 2000

- End-fittings are not included.
- A column connection kit is available separately to ensure proper connections.
- Please refer to the below ordering information.

Description	I.D. (mm)	Length (mm)	Qty	Cat. No.
MonoCap C18 HighResolution 2000	10 $\mu\text{m}$	2000	1/pk	5020-10015

### MonoCap HILIC-UP HighResolution 2000


- End-fittings are not included.
- A column connection kit is available separately to ensure proper connections.
- Please refer to the below ordering information.

Description	I.D. (mm)	Length (mm)	Qty	Cat. No.
MonoCap HILIC-UP HighResolution 2000	10 $\mu\text{m}$	2000	1/pk	5020-10019

### Connection Kit for MonoCap HighResolution 2000

- A dedicated connection kit for MonoCap C18 High Resolution 2000.
- Use this connection kit when connecting the column directly to the system.

Description	Qty	Cat. No.
1/16" PEEK Ferrule, SUS Nut, Sleeve, 2 pcs each.	1/pk	5020-10017
1/32" PEEK Ferrule, SUS Nut, Sleeve, 2 pcs each.		

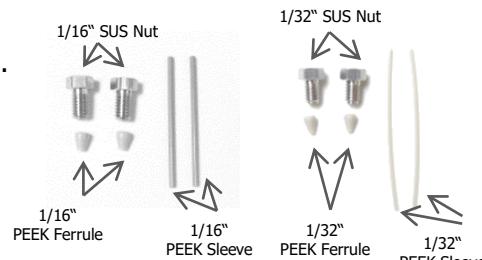

### Zero Dead Volume Union

- Connect the tubing from the system to this union and install the column to achieve zero dead volume.

Description	Orifice Size	Qty	Cat. No.
U-435	0.25 mm	1/pk	6010-72352
U-411	178 $\mu\text{m}$	1/pk	6010-72351




## MonoCap C18 Fast-Flow

### Physical Properties

Product Description	Bonded Phase	Meso-pore	End-capping	Max. Operating Pressure
MonoCap C18 Fast-flow	Octadecyl Groups	15 nm	Yes	22 MPa

Workable at a broad range of linear velocity from 0.5 to 5 mm/s without sacrificing efficiency and separation at high speed. The number of theoretical plates produced by MonoCap C18 Fast-Flow is nearly equivalent to a totally porous particle type capillary column packed with a 5  $\mu$ m packing material. Columns are protected by either metal or PEEK hardware.

#### Workable at High Flow Rates without Sacrificing Efficiency

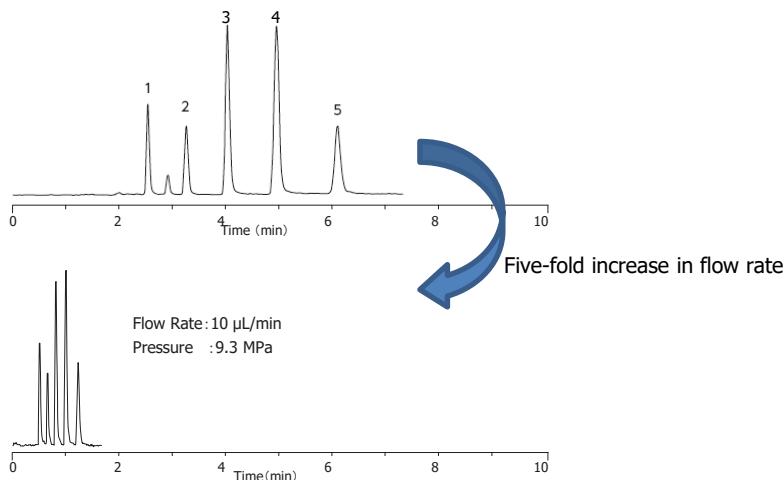

#### Conditions

Column : MonoCap C18 for Fast-flow (150  $\times$  0.2 mm I.D.)  
 Eluent : A)CH<sub>3</sub>CN B) H<sub>2</sub>O  
 A/B=50/50 ,v/v  
 Col.Temp. : Ambient  
 Detection : UV 210 nm (MU701, Cell Volume 18 nL)  
 Injection Vol. : 0.5  $\mu$ L  
 Sample :  
 1. Thiourea  
 2. Acetophenone  
 3. Benzene  
 4. Toluene  
 5. Naphthalene



## Other MonoCap Series

### MonoCap C18 Nano-flow



#### Physical Properties

Product Description	Bonded Phase	Meso-pore	End-capping	Max. Operating Pressure
MonoCap C18 Nano-flow	Octadecyl Groups	11 nm	Yes	22 MPa

MonoCap C18 Nano-flow produces higher number of theoretical plates compared to a totally porous particle type capillary column packed with a 3  $\mu\text{m}$  packing material. It can be operated at a wide range of flow rate with low back pressure and achieve very high sensitive results in Nano-LC-ESI/MS applications. Columns are protected by either metal or PEEK hardware.

### MonoCap C18 WideBore



#### Physical Properties

Product Description	Bonded Phase	Meso-pore	End-capping	Max. Operating Pressure
MonoCap C18 WideBore	Octadecyl Groups	11 nm	Yes	22 MPa

The MonoCap C18 Fast-flow is also available in 0.5 mm I.D. size, which can be used at a wide range of flow rate from 6 to 100  $\mu\text{L}/\text{min}$  without sacrificing efficiency. The number of theoretical plates produced by MonoCap C18 WideBore is nearly equivalent to a totally porous particle type capillary column packed with a 5  $\mu\text{m}$  packing material. Columns are protected by a metal hardware.

### MonoCap C18 Trap Column

#### Physical Properties

Product Description	Bonded Phase	Meso-pore	End-capping	Max. Operating Pressure
MonoCap C18 Trap Column	Octadecyl Groups	11 nm	Yes	20 MPa

MonoCap C18 Trap columns have a relatively big throughpore and workable at a high flow rate such as 10  $\mu\text{L}/\text{min}$ . This benefit makes MonoCap C18 Trap columns to be appropriate for on-line preconcentration or desalting of protein and peptide samples prior to HPLC separation with mass spectrometry detection. End-fittings are 1/16" (10-32 UNF). 1/32" end-fittings are also available upon request.





## MonoCap Amide

### Physical Properties

Product Description	Bonded Phase	Meso-pore	End-capping	Max. Operating Pressure
MonoCap Amide	Carbamoyl Groups	15 nm	None	22 MPa

Amide groups are chemically bonded to the monolithic silica and makes it suitable for the analysis of sugars via HILIC mode. As the back pressure is significantly low, a 500 mm length MonoCap Amide column deliver over 40,000 plates offering high efficiency. Generally, HILIC mode uses acetonitrile at a concentration between 65-95 % in an aqueous buffer such as ammonium acetate or ammonium formate, which have high solubility in organic solvents. Columns are protected by either metal or PEEK hardware.

## MonoCap SCX

### Physical Properties

Product Description	Bonded Phase	Meso-pore	End-capping	Max. Operating Pressure
MonoCap SCX	Benzenesulfonyl Groups	11 nm	None	20 MPa

MonoCap SCX is bonded with benzene sulfonic acid groups (strong cation exchange) and appropriate for 2D LC applications for the separation of biomolecules such as peptides and proteins.



# Other MonoCap Series

## Ordering Information

---

### MonoCap C18 Fast-Flow

- For end-fittings information, please refer to page 30.
- All 50 mm length PEEK columns does not come with a hardware and will be supplied with 3 pcs of columns only.

Description	I.D. (mm)	Length (mm)	Hardware	Qty	Cat. No.
MonoCap C18 Fast-Flow	0.05	50		1/pk	5020-10102
		150	Metal	1/pk	5020-10101
		250		1/pk	5020-10100
		50		3/pk	5020-10002
		150	PEEK	1/pk	5020-10001
	0.075	250		1/pk	5020-10000
		50		1/pk	5020-10211
		150	Metal	1/pk	5020-10212
		250		1/pk	5020-10213
		50		3/pk	5020-10221
	0.1	150	PEEK	1/pk	5020-10222
		250		1/pk	5020-10223
		50		1/pk	5020-10112
		150	Metal	1/pk	5020-10111
		250		1/pk	5020-10110
	0.2	50		3/pk	5020-10012
		150	PEEK	1/pk	5020-10011
		250		1/pk	5020-10010
		50		1/pk	5020-10122
		150	Metal	1/pk	5020-10121
		250		1/pk	5020-10120
		50		3/pk	5020-10022
		150	PEEK	1/pk	5020-10021
		250		1/pk	5020-10020

## Ordering Information

---

### MonoCap C18 Nano-Flow

- For end-fittings information, please refer to page 30.
- All 50 mm length PEEK columns does not come with a hardware and will be supplied with 3 pcs of columns only.

Description	I.D. (mm)	Length (mm)	Hardware	Qty	Cat. No.
MonoCap C18 Nano-Flow	0.05	50	Metal	1/pk	5020-10143
		150		1/pk	5020-10141
		50	PEEK	3/pk	5020-10043
		150		1/pk	5020-10041
	0.075	50	Metal	1/pk	5020-10231
		150		1/pk	5020-10232
		50	PEEK	3/pk	5020-10241
		150		1/pk	5020-10242
	0.1	50	Metal	1/pk	5020-10153
		150		1/pk	5020-10151
		50	PEEK	3/pk	5020-10053
		150		1/pk	5020-10051
	0.2	50	Metal	1/pk	5020-10163
		150		1/pk	5020-10161
		50	PEEK	3/pk	5020-10063
		150		1/pk	5020-10061

### MonoCap C18 WideBore

- For end-fittings information, please refer to page 30.

Description	I.D. (mm)	Length (mm)	Hardware	Qty	Cat. No.
MonoCap C18 WideBore	0.5	50	Metal only	1/pk	5020-10202
		150		1/pk	5020-10201
		250		1/pk	5020-10200

# Other MonoCap Series

## Ordering Information

### MonoCap C18 Trap Column

- For end-fittings information, please refer to page 30.

Description	I.D. (mm)	Length (mm)	Hardware	Qty	Cat. No.
MonoCap C18 Trap Column	0.05	50		1/pk	5020-10026
		100	With Hardware	1/pk	5020-10038
		150		1/pk	NA
		50		1/pk	5020-10027
		100	Without Hardware	1/pk	5020-10039
	0.075	150		1/pk	NA
		50		1/pk	5020-10028
		100	With Hardware	1/pk	5020-10036
		150		1/pk	NA
		50		1/pk	5020-10029
	0.2	100	Without Hardware	1/pk	5020-10037
		150		1/pk	NA
		50		1/pk	5020-10033
		100	With Hardware	1/pk	NA
		150		1/pk	NA
		50		1/pk	5020-10034
		100	Without Hardware	1/pk	NA
		150		1/pk	5020-10031

### MonoCap Amide

- For end-fittings information, please refer to page 30.

Description	I.D. (mm)	Length (mm)	Hardware	Qty	Cat. No.
MonoCap Amide	0.075	150		1/pk	5020-10191
		250	Metal	1/pk	5020-10192
		500		1/pk	5020-10193
		150		1/pk	5020-10091
		250	PEEK	1/pk	5020-10092
	0.1	500		1/pk	5020-10093
		150		1/pk	5020-10181
		250	Metal	1/pk	5020-10182
		500		1/pk	5020-10183
		150		1/pk	5020-10081
	0.2	250	PEEK	1/pk	5020-10082
		500		1/pk	5020-10083
		150		1/pk	5020-10171
		250	Metal	1/pk	5020-10172
		500		1/pk	5020-10173
	0.25	150		1/pk	5020-10071
		250	PEEK	1/pk	5020-10072
	0.32	500		1/pk	5020-10073

## Ordering Information

---

### MonoCap SCX

- For end-fittings information, please refer to the following information.

Description	I.D. (mm)	Length (mm)	Hardware	Qty	Cat. No.
MonoCap SCX	0.2	50	Metal	1/pk	5020-10174
		150		1/pk	5020-10175
		250		1/pk	5020-10176
		500		1/pk	5020-10177
	0.2	50	PEEK	1/pk	5020-10074
		150		1/pk	5020-10075
		250		1/pk	5020-10076
		500		1/pk	5020-10077

### End-fittings of MonoCap Monolithic Capillary HPLC Columns

Description	End-fittings Details
MonoCap C18 Fast-flow	1. Metal Hardware Type End-fittings are Valco 1/16" (10-32 UNF).
MonoCap C18 Nano-flow	Valco 1/32" (6-40 UNF) end-fittings can also be arranged upon request, indicate "1/32" when ordering.
MonoCap C18 WideBore	
MonoCap Amide	
MonoCap SCX	2. PEEK Hardware Type 1/16" male nut, ferrule and PTFE sleeve are included.

### Connection Kit for MonoCap C18 Trap Column

Description	Cat. No.
MonoCap C18 Trap Column Connection Kit 1/16" (Union·Sleeve·Capillary Tubing 2 pcs each, Nut·Ferrule 4 pcs each)	5020-10044
MonoCap C18 Trap Column Connection Kit 1/32" (Union·Sleeve·Capillary Tubing 2 pcs each, Nut·Ferrule 4 pcs each)	5020-10045
MonoCap C18 Trap Column Assembly Parts 1/16" (Nut·Ferrule 4 pcs each)	5020-10046
MonoCap C18 Trap Column Assembly Parts 1/32" (Nut·Ferrule 4 pcs each)	5020-10047



## MonoSpray

### Monolithic Electrospray Emitter for ESI-LC/MS

---

MonoSpray is an electrospray emitter for ESI-LC/MS which a monolithic packing is packed into a fused silica sprayer offering numbers of benefits compared to those traditional sprayers packed with particle based packings. Frits are not installed in MonoSpray to keep the monolithic packing in place, which results in offering simply longer lifetime and avoiding bed splitting problems compared to those traditional sprayers packed with particle based packings. The very high porosity of monolithic packing allows a wide range of operational flow rates, even at high flow rates.

### Features

---

- High Sensitivity Analysis
- High Chemical Stability
- High Physical Stability
- Wide Range of Operational Flow Rates

### Ordering Information

---

#### MonoSpray FS

- For online Nano-ESI-LC/MS.

Description	Length (mm)	O.D. (µm)	I.D. (µm)	Qty	Optimum Flow Rate	Cat. No.
MonoSpray FS	50	370	50	5 pcs	0.1 - 1.0 µL/min	5010-20001
				20 pcs		5010-20006
			75	5 pcs	0.2 - 2.0 µL/min	5010-20002
				20 pcs		5010-20007
			100	5 pcs	1.0 - 5.0 µL/min	5010-20003
				20 pcs		5010-20008

Please inquire for other sizes.

#### MonoSpray C18 Nano

- Nano sprayer packed with octadecylated silica monolith offering reversed phased separation.

Description	Length (mm)	O.D. (µm)	I.D. (µm)	Qty	Optimum Flow Rate	Cat. No.
MonoSpray C18 Nano	50	370	50	1 pcs	0.1 - 0.5 µL/min	5010-20011
				4 pcs		5010-20016
			75	1 pcs	0.1 - 1.0 µL/min	5010-20012
				4 pcs		5010-20017
			100	1 pcs	0.3 - 2.0 µL/min	5010-20013
				4 pcs		5010-20018

Please inquire for other sizes.


# MonoSpin Series

## Low-Molecular Compounds Extraction and Purification

The low-pressure, high-flow, and low-liquid-retention properties of GL Sciences' monolith silica technology make it uniquely suited for handling of small samples. MonoSpin SPE centrifugal spin columns have been developed to improve concentration and yields in low-volume sample preparation.


### Features

- Easy-to-Operate
- Ideal for Small Sample Volumes
- Wide Variety of Functional Groups
- Rapid Operation Time

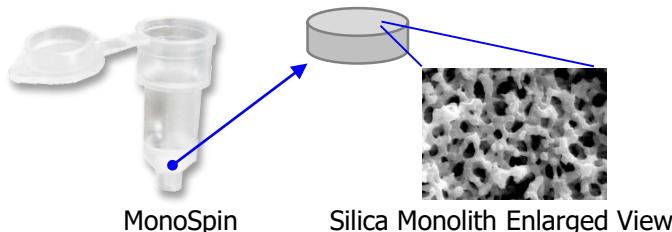


### How to Operate

Centrifuge elution allows loss-free and efficient processing of many samples simultaneously, with little or no liquid retained by the separation matrix. And, excellent mass transfer and rapid sample binding on MonoSpin's monolith silica allows extremely rapid sample preparation compared with other methods.

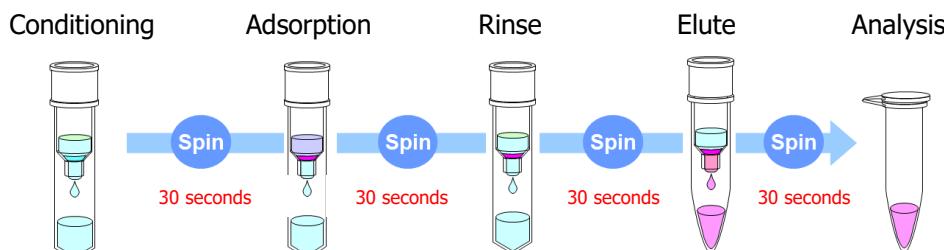

### Formats



#### S Type (Small)

- Disc Size :  $\phi 4.2 \times 1.5$  mm
- Sample Volume : 50 ~ 800  $\mu$ L
- Elution Volume : 50 ~ 800  $\mu$ L
- Centrifugation Speed : 2,000 ~ 10,000  $\times g$




#### L Type (Large)

- Disc Size :  $\phi 9 \times 3$  mm
- Sample Volume : 0.5 ~ 8 mL
- Elution Volume : 0.5 ~ 8 mL
- Centrifugation Speed : 1,000  $\times g$

## Product Lineup


### MonoSpin C18/C18 FF



Formats: S L

Octadecyl functional group. Optimal for drug extraction in biological samples, and desalting & enrichment of peptide samples C18 FF type employs large through-pore monolith silica for high viscosity samples.


### MonoSpin C18-AX



Formats: S

Bonded with octadecyl and trimethylaminopropyl, a mix mode type. Delivers great retention for high salt concentrated serum samples. Optimal for the recovery of acidic drugs.


### MonoSpin SAX



Formats: S L

Bonded with trimethylaminopropyl combining both strong anion exchange & weak hydrophobic interaction. Optimal for the extraction of acidic drugs.


### MonoSpin NH2



Formats: S L

Bonded with aminopropyl. Optimal for the enrichment of sugar chain and/or hydrophilic compounds by HILIC mode.


### MonoSpin Amide



Formats: S

Bonded with amide. Optimal for the extraction of sugar chains and various hydrophilic acidic and basic compounds by HILIC mode.

### MonoSpin TiO




Formats: S

Monolith skeleton coated with titanium dioxide. Excellent for the enrichment of phosphopeptides.

S : Small Type L : Large Type

## Product Lineup

### MonoSpin ME



Formats: S L

Bonded with iminodiacetic acid. Optimal for the recovery of trace metals.



### MonoSpin Ph



Formats: S

Phenyl functional group. Optimal for the recovery of hydrophobic drugs in biological samples due to its weak retentivity and different selectivity compared to a C18 phase.



### MonoSpin C18-CX



Formats: S

Bonded with octadecyl and benzene sulfonic acid combining both ion exchange & hydrophobic interaction. Optimal for dissociated basic drug in biological samples. Delivers higher cleanup efficiency compared to C18 or SCX.


### MonoSpin SCX



Formats: S L

Bonded with benzenesulfonic acid combining both strong cation exchange & hydrophobic interaction. Optimal for the extraction of basic drugs.



### MonoSpin CBA



Formats: S L

Bonded with carboxyl acid combining both weak cation exchange. Optimal for the extraction of basic drugs.

### MonoSpin PBA



Formats: S

Specific column combined with phenyl boric acid. Excellent for the selective extraction of cis diol compounds, such as catechol amines.

S : Small Type

L : Large Type


## Product Lineup

---

### MonoSpin Trypsin

Formats: S


Immobilized trypsin is available for performing rapid and efficient tryptic digests of proteins.



### MonoSpin Phospholipid

Formats: S L


Monolith skeleton coated with TiO<sub>2</sub> and ZrO<sub>2</sub>. Excellent for the adsorption and removal of phospholipids.



### MonoSpin ProA

Formats: S 96


Protein A immobilized affinity spin column for the rapid purification of antibodies.



### MonoSpin ProG

Formats: S 96

Protein G immobilized affinity spin column for the rapid purification of antibodies.



S : Small Type   L : Large Type   96 : 96-well plate

## Physical Properties

Product	Stationary Phases	S Type (Small)		L Type (Large)		Surface Area (m <sup>2</sup> /g)	Sample Loading Capacity (Small Type)	Filter
		Through-pore (μm)	Meso-pore (nm)	Through-pore (μm)	Meso-pore (nm)			
MonoSpin C18	Octadecyl	5	10	10	10	350	100 μg (Amitriptyline)	None
MonoSpin C18 FF	Octadecyl	20	15	-	-	300	50 μg (Amitriptyline)	
MonoSpin Ph	Phenyl	5	10	-	-	350	100 μg (Amitriptyline)	
MonoSpin C18-AX	Octadecyl, Trimethylaminopropyl	5	10	-	-	350	100 μg (Ibuprofen)	
MonoSpin C18-CX	Octadecyl, Benzenesulfonic acid	5	10	-	-	350	100 μg (Amitriptyline)	
MonoSpin SAX	Trimethylaminopropyl	5	10	10	10	350	100 μg (Ibuprofen)	
MonoSpin SCX	Benzenesulfonic acid	5	10	10	10	350	100 μg (Amitriptyline)	
MonoSpin NH2	Aminopropyl	5	10	10	10	350	100 μg (Maltopentaose)	
MonoSpin CBA	Carboxyl	5	10	10	10	350	100 μg (Amitriptyline)	
MonoSpin Amide	Amide	5	10	-	-	350	100 μg (Angiotensin II)	
MonoSpin PBA	Phenyl boric acid	5	10	-	-	350	100 μg (Dopamine)	
MonoSpin TiO	Titanium dioxide	20	15	-	-	350	40 μg (Adenosine monophosphate)	
MonoSpin Trypsin	TPCK treated Trypsin	5	10	-	-	350	-	
MonoSpin ME	Iminodiacetic acid	5	10	10	10	350	25 μg (Cu ion)	
MonoSpin Phospholipid	TiO <sub>2</sub> + ZrO <sub>2</sub>	5	10	10	10	350	10 μL (Human serum)	
MonoSpin ProA	Protein A	2	60	-	-	-	400 μg (Human IgG)	
MonoSpin ProG	Protein G	2	60	-	-	-	400 μg (Human IgG)	


## Specifications

Description	MonoSpin S Type * <sup>1</sup>	MonoSpin FF * <sup>2</sup>	MonoSpin L Type
Disc Size	Φ 4.2 x 1.5 mm	Φ4.2 x 1.5 mm	Φ9 x 3 mm
Sample Volume	50 ~ 800 μL	50 ~ 800 μL	0.5 ~ 8 mL
Elution Volume	50 ~ 800 μL	50 ~ 800 μL	0.5 ~ 8 mL
Centrifugation Speed	2,000~10,000 x g	1,000 x g	1,000 x g
Sample Loading Capacity	100 μg	50 μg	1 mg



## Appropriate for Various Viscosity Samples

MonoSpin series are ideal for the sample preparation of biological samples. MonoSpin C18 Fast Flow (FF) type is excellent for high viscosity biological samples. Select the appropriate MonoSpin column type depending on the viscosity of sample and volume.

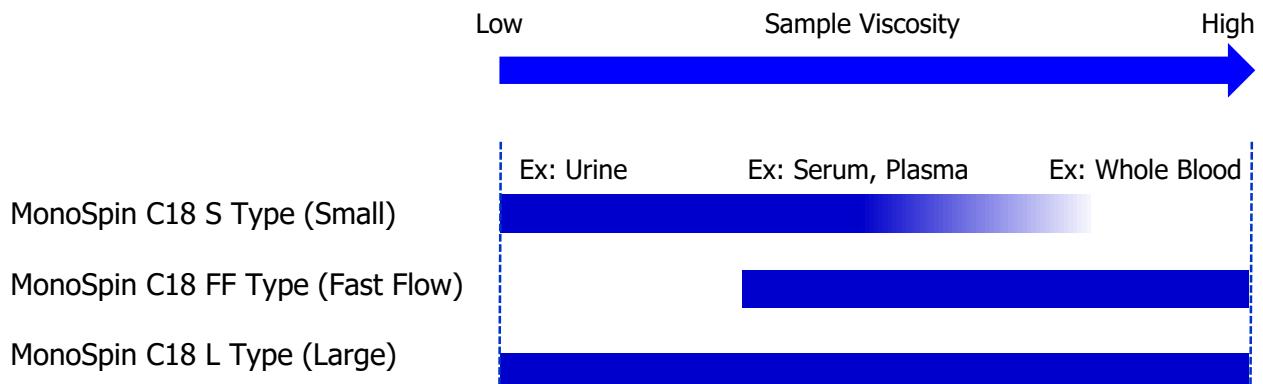


## MonoSpin Applications

The low-pressure, high-flow, and low-liquid-retention properties of GL Sciences' monolith silica technology make it uniquely suited for handling of small samples. MonoSpin SPE centrifugal spin columns have been developed to improve concentration and yields in low-volume sample preparation without requiring evaporation or reconstitution.

### Purification and Enrichment of Trace Samples

Without MonoSpin PBA




#### Purification using MonoSpin PBA S Type (Small)

Sample Volume : 500  $\mu$ L

Elution Volume : 500  $\mu$ L

Elution Volume : 50  $\mu$ L  
(10-fold concentration)



#### Conditions



Column : Inertsil ODS-3 (5  $\mu$ m, 150 mm  $\times$  2.1 mm I.D.)  
Eluent : 50 mM Phosphate buffer (pH 5.6)  
50 mg/L EDTA  
600 mg/L IPCC-008  
-10 % Methanol  
Flow Rate : 0.3 mL/min  
Col.Temp. : 35 °C  
Injection : 5  $\mu$ L  
Detection : ECD Pulse Mode  
Sample :  
1. Noradrenaline  
2. Adrenaline  
3. DHBA  
4. Dopamine

Without MonoSpin C18

#### Purification of Serum using MonoSpin C18 L Type (Large)

Sample Volume : 5000  $\mu$ L

Elution Volume : 500  $\mu$ L  
(10-fold concentration)

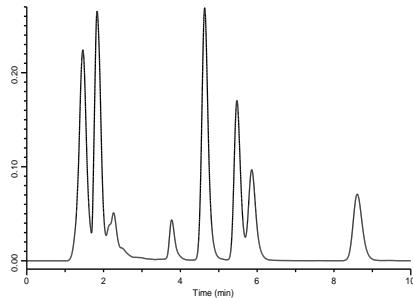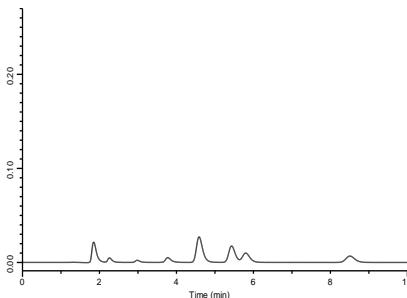

5000  $\mu$ L serum sample is purified with MonoSpin C18 and enriched by 500  $\mu$ L.

#### Conditions

Column : Inertsil ODS-3 (5  $\mu$ m, 150  $\times$  4.6 mm I.D.)  
Eluent : CH<sub>3</sub>CN/3 mM KH<sub>2</sub>PO<sub>4</sub>, 27 mM SDS=48=52  
Flow Rate : 1.0 mL/min

Col.Temp : 40 °C  
Injection Vol. : 1  $\mu$ L  
Detection : 230 nm



# MonoSpin Series

## Purification of Amphetamine in Urine using MonoSpin C18

### Sample Preparation

800  $\mu$ L sample solution mixed with 400  $\mu$ L urine and 400  $\mu$ L buffer solution (pH 13.0).

Centrifugation Speed: 5,000  $\times$  g

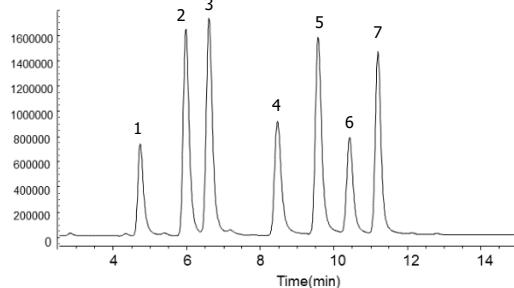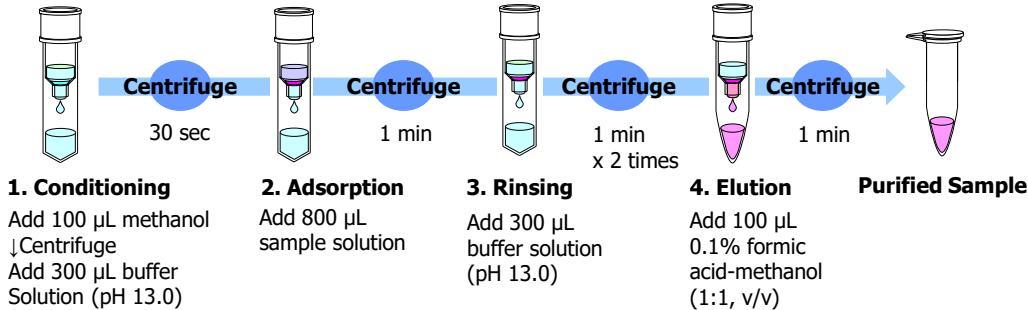

### Conditions

Column : InertSustainSwift C18 (3  $\mu$ m, 150  $\times$  2.1 mm I.D.)  
 Eluent : A) 10 mM Ammonium acetate-Formic acid (pH 3.3)  
 B)  $\text{CH}_3\text{OH}$   
 A/B = 90/10 - 2 min - 90/10 - 13 min - 70/30, v/v  
 Flow Rate : 0.3 mL/min  
 Col. Temp. : 40 °C  
 Detection : LC/MS  
 Sample :  
 1. Norephedrine  
 2. Ephedrine  
 3. Methylephedrine  
 4. Amphetamine  
 5. Methamphetamine  
 6. 3,4-methylenedioxymethamphetamine  
 7. 3,4-methylenedioxymethamphetamine


※ Data provided from Hiroshima University, Dr. Namera

## Recovery of Drugs in Serum using MonoSpin C18

### Sample Preparation

600  $\mu$ L sample solution mixed with 200  $\mu$ L serum and 400  $\mu$ L 10 mM potassium phosphate buffer solution (pH 7.0).

Centrifugation Speed: 2,300  $\times$  g

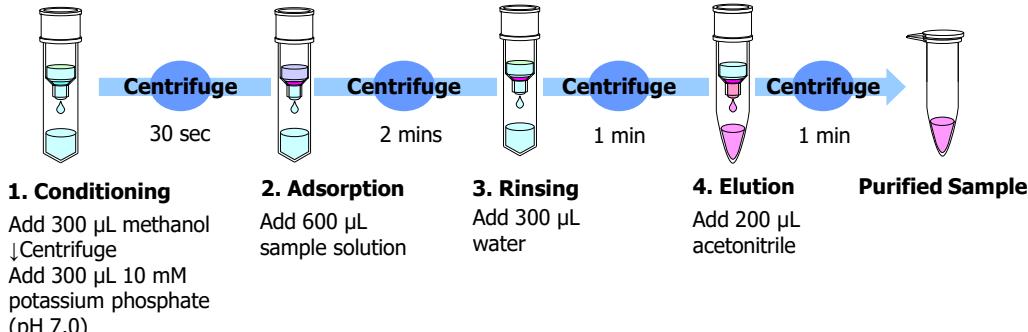

**Reproducibility study for drugs in serum sample for three days using MonoSpin C18 (n=10)**  
**MonoSpin demonstrated high reproducibility for purification of drugs.**

Sample	Con. (ng/mL)	Rec. (%)	RSD (%)
Desipramine	5	91.2	4.8
	10	86.1	3.3
	50	85.2	5.9
	250	88.4	6.5
Imipramine	5	96.3	9.5
	10	95.8	1.5
	50	94.5	0.9
	250	95.9	0.9
Fluvoxamine	5	96.8	11.6
	10	87.1	5.0
	50	86.8	8.1
	250	87.5	9.7

Sample	Con. (ng/mL)	Rec. (%)	RSD (%)
Paroxetine	5	83.7	3.9
	10	84.1	7.8
	50	83.9	8.2
	250	86.7	7.5
Maprotiline	5	85.7	8.1
	10	84.7	3.2
	50	88.6	5.4
	250	87.5	7.7
Duloxetine	5	106.3	9.9
	10	104.8	6.7
	50	99.8	8.7
	250	99.8	6.0


Sample	Con. (ng/mL)	Rec. (%)	RSD (%)
Amitriptyline	5	83.7	7.0
	10	81.8	2.8
	50	83.8	3.0
	250	88.4	2.7
Sulpiride	5	97.9	9.0
	10	95.5	8.5
	50	90.8	2.6
	250	92.6	3.0

## Desalting of Protein Digests using MonoSpin C18


### Sample Preparation

800  $\mu$ L sample solution:  
Add TFA to tryptic digest sample and adjust the TFA final concentration to 0.1%.


Centrifugation  
Speed: 2,300  $\times$  g

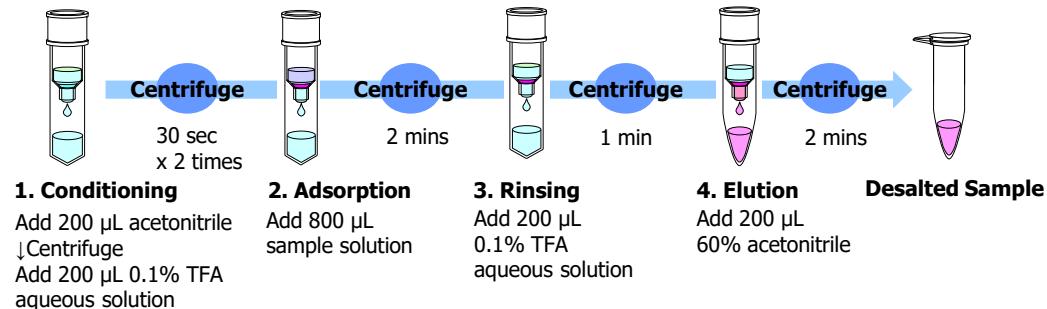

Without MonoSpin C18

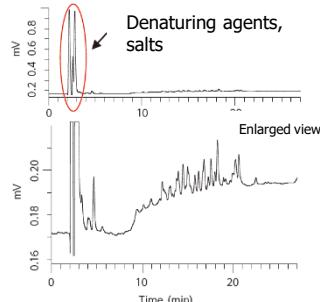

Desalting using MonoSpin C18

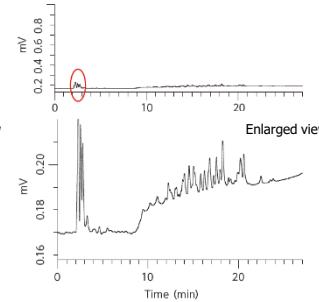

### Conditions


Column : Inertsil ODS-3  
(3  $\mu$ m, 150  $\times$  2.1 mm I.D.)  
Eluent : A)  $\text{H}_2\text{O}$  (0.1 % TFA)  
B) Acetonitrile (0.1 % TFA)  
A/B = 90/10 - 20 min - 50/50  
Flow Rate : UV 210 nm  
Col. Temp. : 0.2 mL/min  
Detection : 40 °C  
Sample : Digested BSA 2  $\mu$ L

## Recovery of Hormone in Serum using MonoSpin C18


### Sample Preparation

Add 20  $\mu$ L of 1 mg/mL of Adrenomedullin to 190  $\mu$ L of serum. Add 0.1% TFA to the serum solution and centrifuged at 10,000  $\times$  g for 1 min. Take the supernatant.

Centrifugation  
Speed: 2,300  $\times$  g

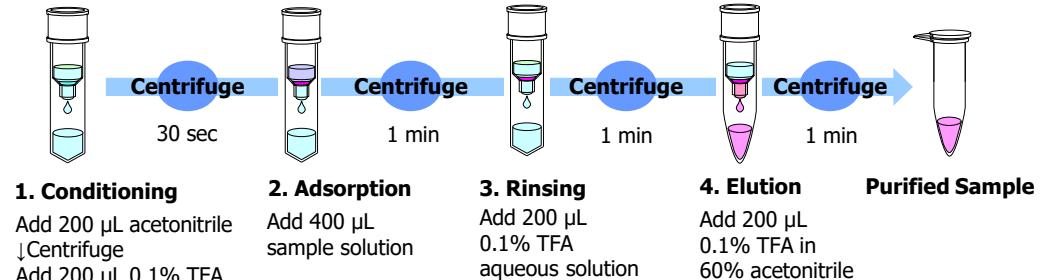

Adrenomedullin

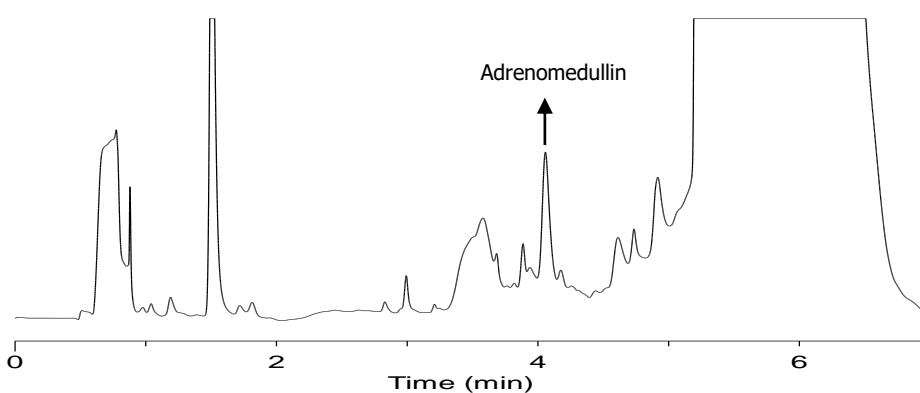

### Conditions

Column : InertSustain C18  
(2  $\mu$ m, 50  $\times$  2.1 mm I.D.)  
Eluent : A) 0.1 % TFA in  $\text{H}_2\text{O}$   
B) 0.1 % TFA in Acetonitrile  
A/B = 85/15 - 5 min - 50/50  
Flow Rate : 200  $\mu$ L/min  
Col. Temp. : 40 °C  
Detection : UV 210 nm  
Injection Vol. : 10  $\mu$ L



# MonoSpin Series

## Purification of Whole Blood using MonoSpin C18 FF (Fast Flow)

### Sample Preparation

Mix 0.3 mL whole blood and 1.2 mL 300 mM phosphate buffer (pH 10). Centrifuge at 12,100  $\times$  g for 5 mins and take the supernatant.

Centrifugation  
Speed: 1,000  $\times$  g

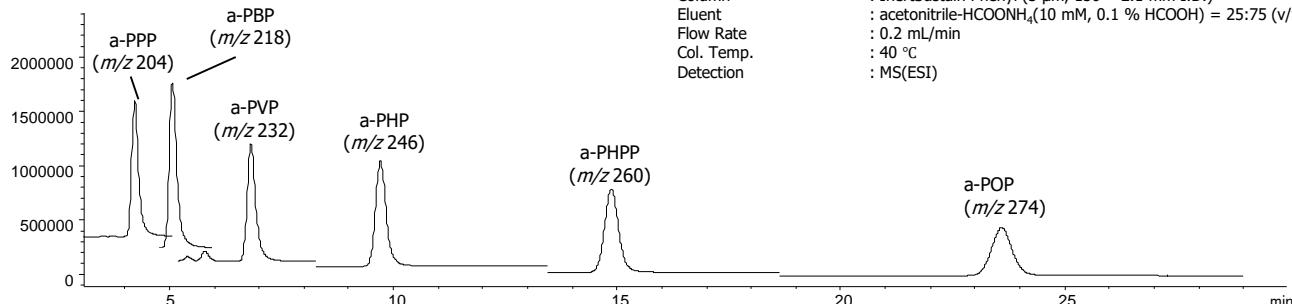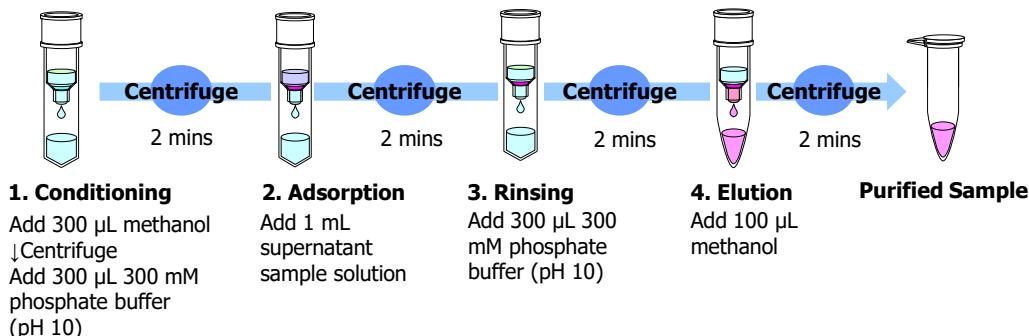

## Features of MonoSpin C18 FF (Fast Flow)

MonoSpin C18 FF is ideal for high viscosity samples, such as whole blood and complex matrix samples.

### Specification

Through-pore	20 $\mu$ m
Meso-pore	15 nm
Disc Size	$\phi$ 4.2 x 1.5 mm
Sample Volume	50 ~800 $\mu$ L
Elution Volume	50 ~800 $\mu$ L
Centrifugation Speed	Under 1,000 $\times$ g
Sample Loading Capacity	50 $\mu$ g (Amitriptyline)

MonoSpin C18 FF offer fast flow of viscosity samples at a low centrifugation speed (1,000  $\times$  g). The following is a comparison of flow of solvents between MonoSpin C18 and MonoSpin C18 FF.

Solvents	Volume	MonoSpin C18	MonoSpin C18 FF
Methanol	500 $\mu$ L	○	○
Water	500 $\mu$ L	400 $\mu$ L	○
Serum*	500 $\mu$ L	300 $\mu$ L	○

**Testing Conditions**  
1,000  $\times$  g 30 sec


\* A supernatant from serum sample was used, which was centrifuged at 10,000  $\times$  g for 1 min.

## Purification of Pyridylaminated (PA) Sugar Chain using MonoSpin NH2

### Sample Preparation


800  $\mu$ L sample solution:  
Add acetonitrile to PA sugar chain sample solution and adjust the acetonitrile final concentration from 90 to 95%.

Centrifugation  
Speed: 2,300  $\times$  g

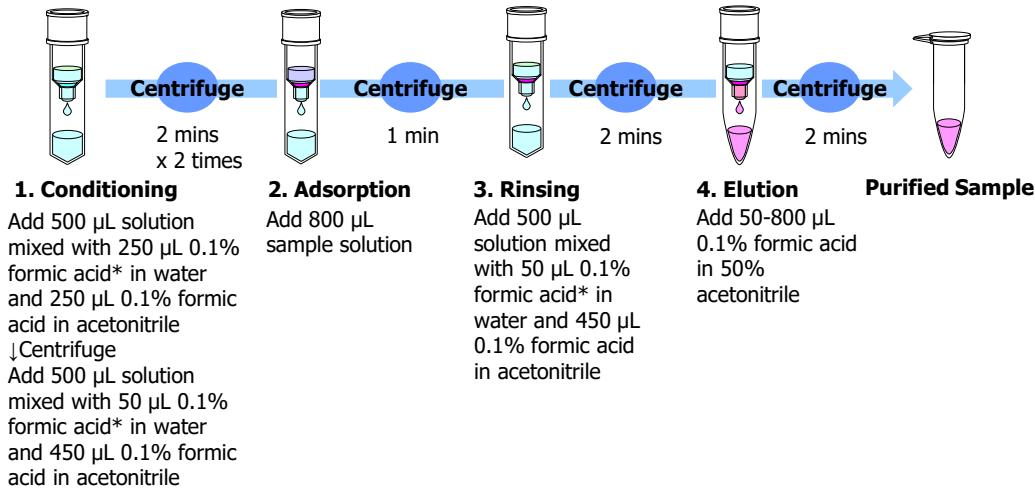


\* Acetic acid or TFA can also be used as an alternative to formic acid.

### Without MonoSpin NH2

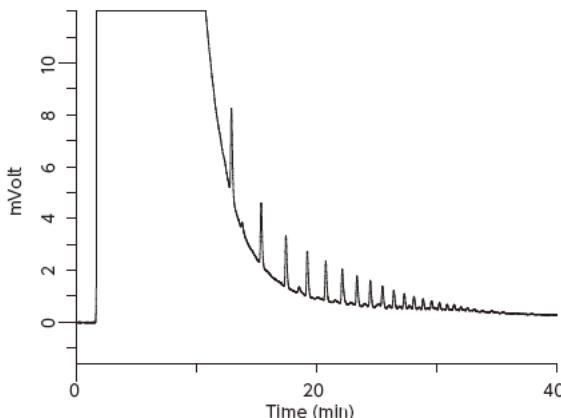

### Purification of PA using MonoSpin NH2

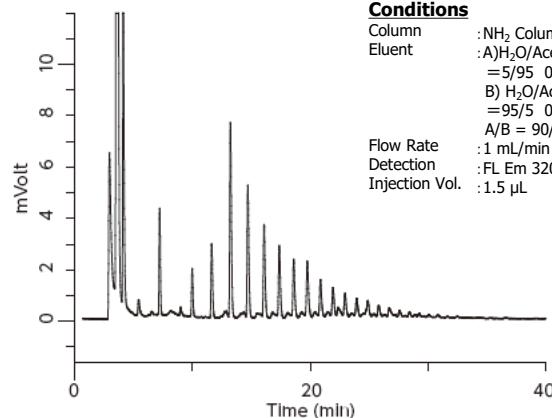


### Conditions

Column : NH<sub>2</sub> Column (5  $\mu$ m, 250  $\times$  4.6 mm I.D.)  
Eluent : A)H<sub>2</sub>O/Acetonitrile = 5/95 0.1 % Formic acid  
B) H<sub>2</sub>O/Acetonitrile = 95/5 0.1 % Formic acid  
A/B = 90/10-10 min-90/10-40 min-60/40  
Flow Rate : 1 mL/min  
Detection : FL Em 320 nm, Ex 400 nm  
Injection Vol. : 1.5  $\mu$ L

**Purified PA sugar chain by HILIC mode.**  
**MonoSpin NH2 additionally removes residual fluorescent labeling reagents.**

## Fractionation of Protein Digests using MonoSpin SCX

MonoSpin SCX provide a rapid and easy fractionation of peptides by stepwise elution using buffers with various salt concentration.

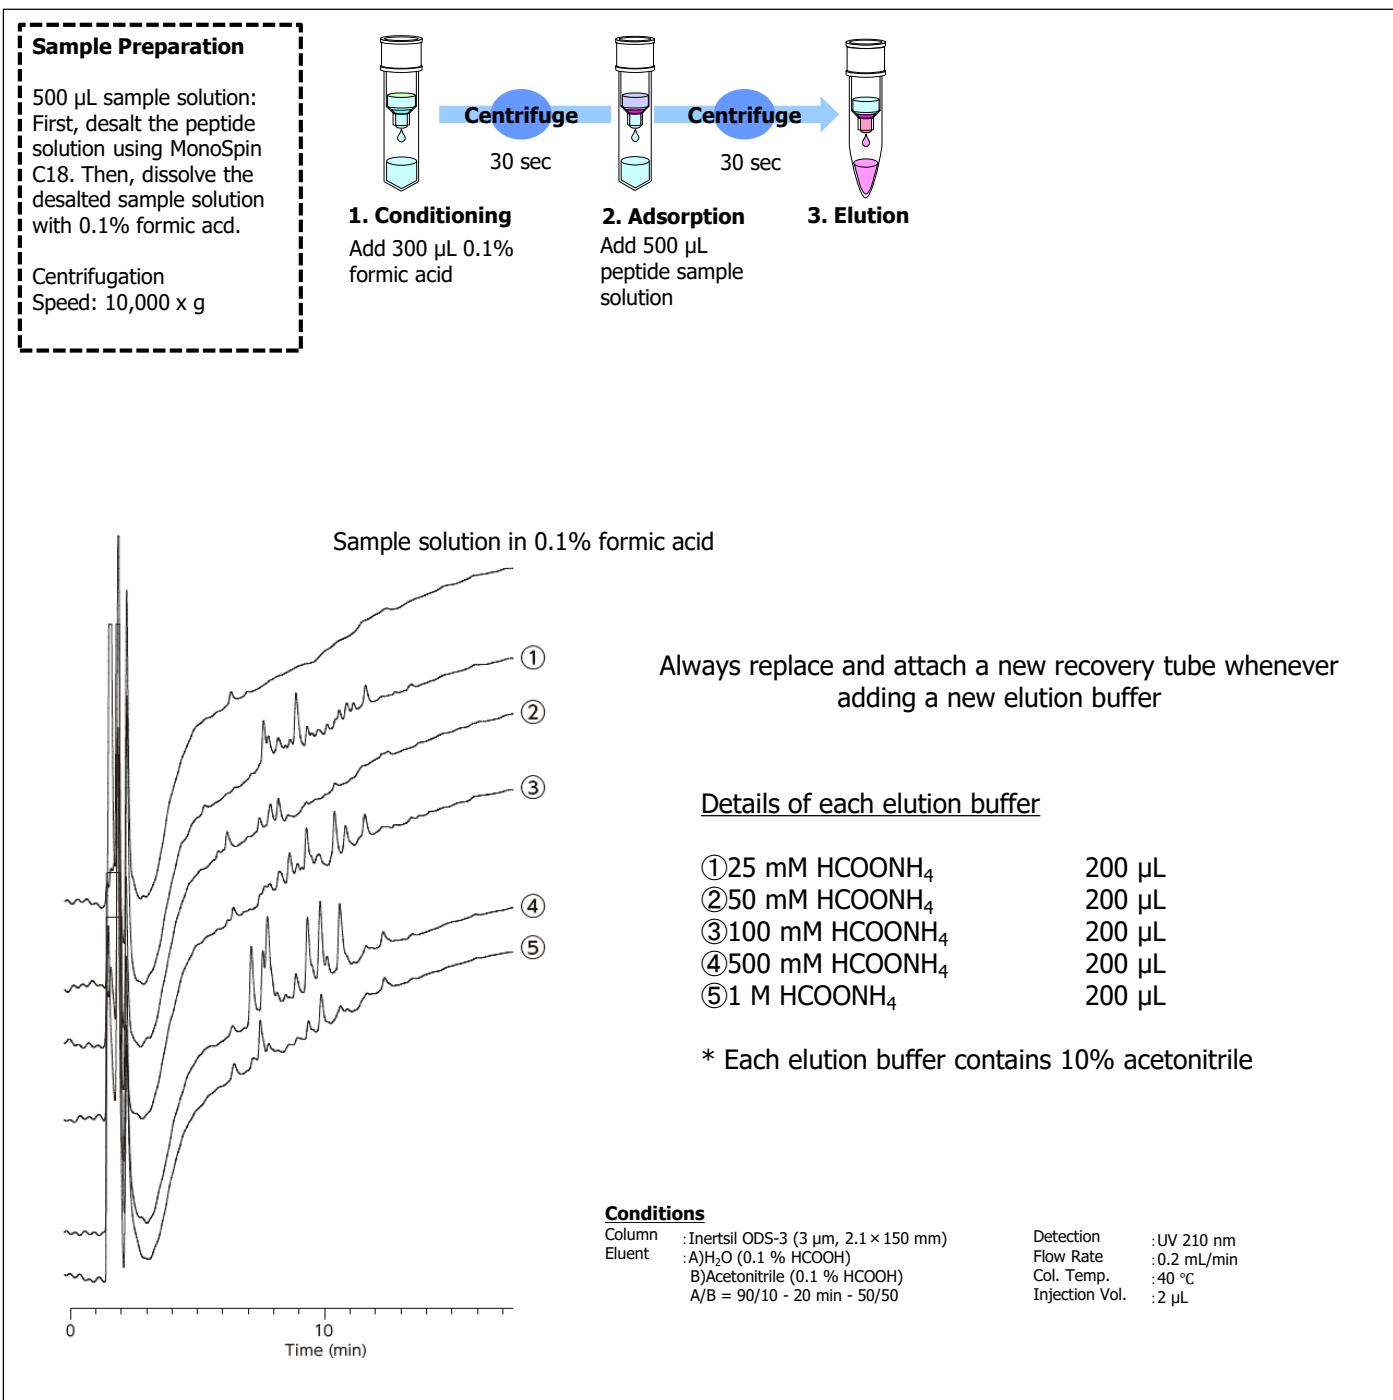


## Purification of Paraquat and Diquat using MonoSpin CBA

### Sample Preparation

600  $\mu$ L sample solution:  
Add 200  $\mu$ L urine and 400  $\mu$ L 10 mM potassium phosphate buffer (pH 7.0)

Centrifugation  
Speed: 10,000  $\times$  g

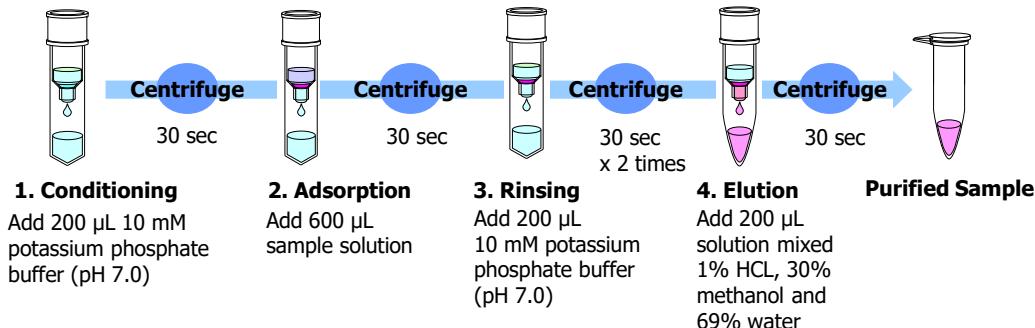


### Conditions


Column : Inertsil ODS-3 (5  $\mu$ m, 150 mm  $\times$  4.6 mm I.D.)  
Eluent : 0.2 M phosphoric acid, 0.1 M diethyl amine, 7.5 mM IPCC08(IPCC-0.8, Sodium 1-Octanesulfonate) /Acetonitrile=89/11

Flow Rate : 1 mL/min  
Col.Temp. : 40  $^{\circ}$ C  
Detection : DAD 290 nm  
Injection Vol. : 50  $\mu$ L


Standard Solution (1  $\mu$ g/mL)

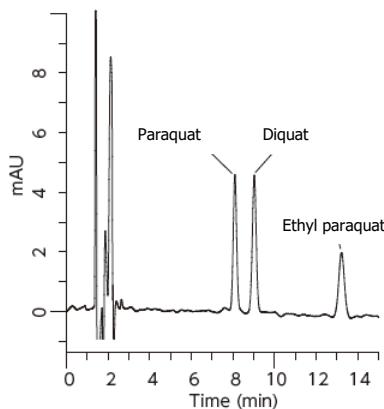

Urine + Pesticide (1  $\mu$ g/mL)

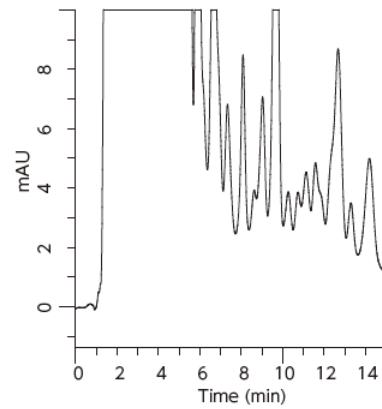


**Purification using MonoSpin CBA**

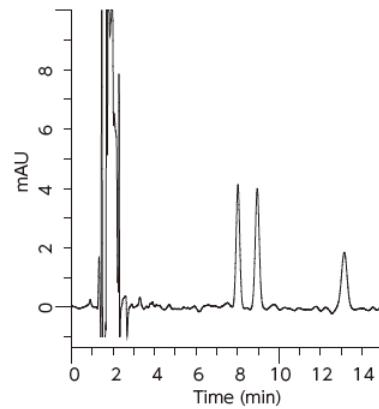


**MonoSpin CBA deliver highly efficient purification of strong basic pesticides such as Paraquat and Diquat.**

# MonoSpin Series

## Purification of Catecholamines using MonoSpin PBA

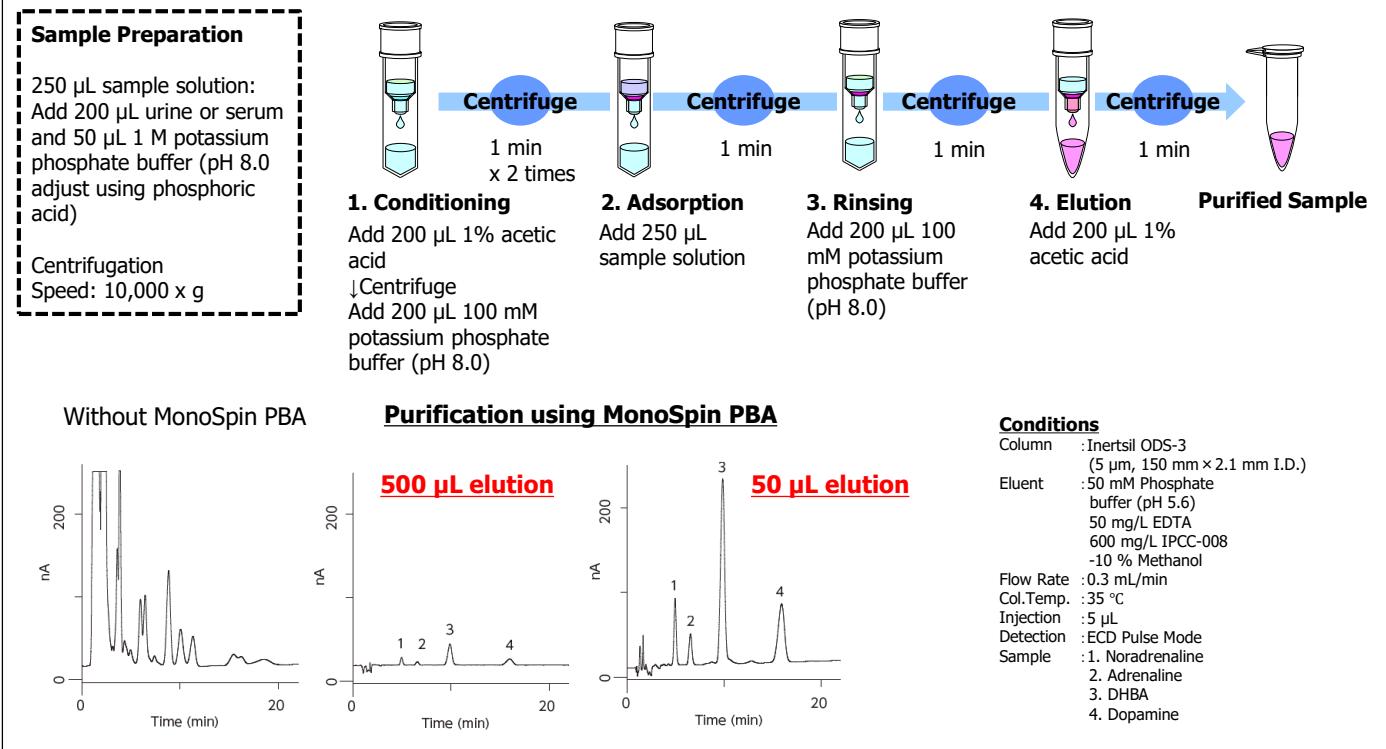

## Purification of Organic Phosphorous Pesticides in Serum using MonoSpin TiO

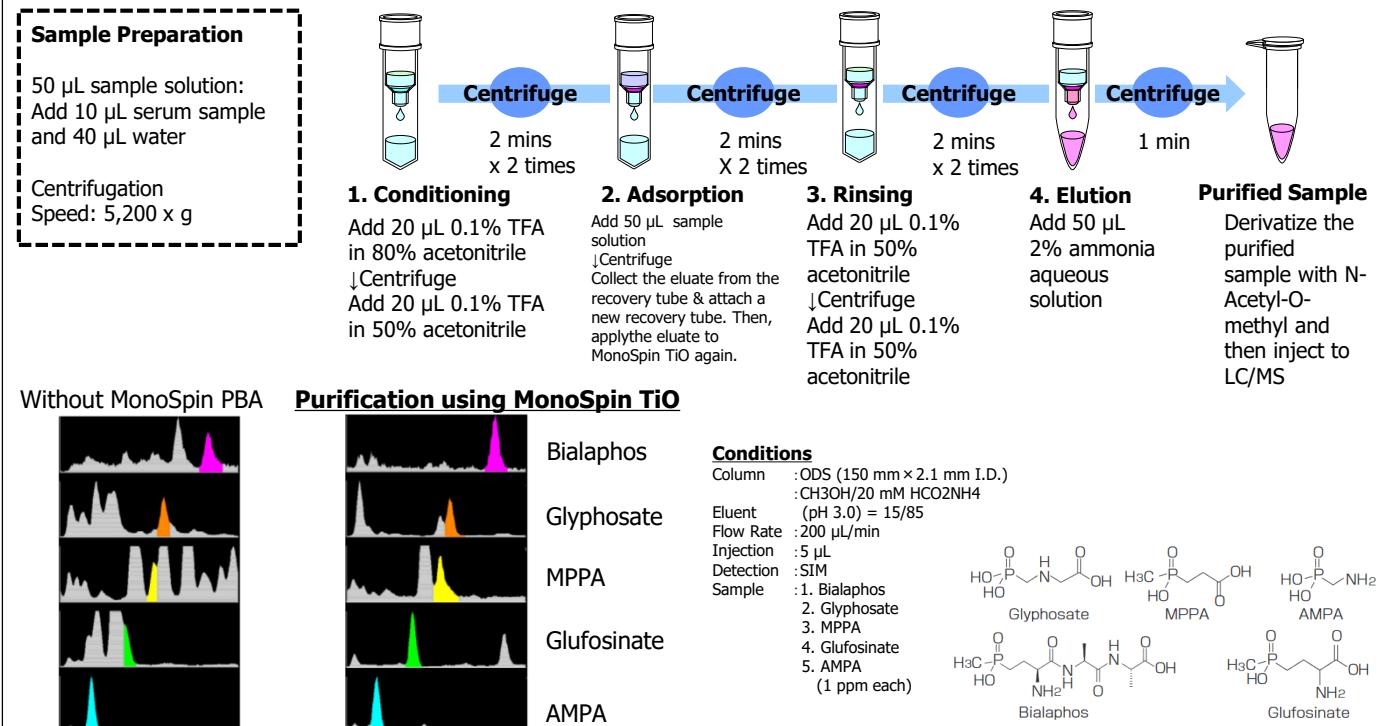

## Rapid Digestion of BSA using MonoSpin Trypsin

### Example of Reduction and Alkylation Protocol

1 mg Bovine serum albumin

- Add 175  $\mu$ L 500 mM Tris-HCL (pH 8.0) and 8 M urea (Solution 1).
- Add 25  $\mu$ L 40 mg/mL dithiothreitol in Solution 1.
- Incubation at 37 °C for 90 mins
- Add 50  $\mu$ L 40 mg/mL iodoacetoamide in Solution 1.
- Incubation at 37 °C for 30 mins without exposure to light.


250  $\mu$ L Reduced and alkylated protein

- Add 50 mM ammonium bicarbonate to make the urea final concentration to 2 M and dilute it to 750  $\mu$ L

### MonoSpin Trypsin



The protocol above is just an example.

Optimize the protocol of preparation of reduced and Alkylated sample depending on the types of proteins.

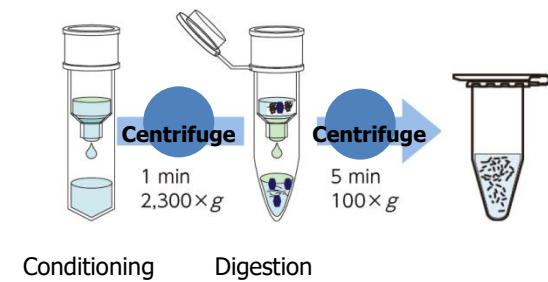

Incubation at 37 °C for 10 hours

### Protein Digestion at 25 °C for 10 minutes using MonoSpin Trypsin

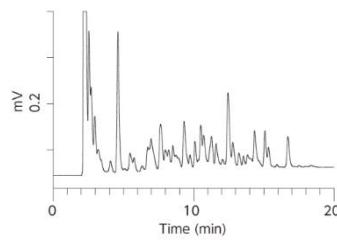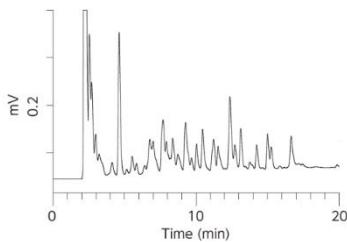

#### Conditions

Column	: Inertsil ODS-3 (3 $\mu$ m, 150 $\times$ 2.1 mm I.D.)
Eluent	: A)H <sub>2</sub> O (0.1 % HCOOH) B)Acetonitrile (0.1 % HCOOH)
Flow Rate	: A/B = 90/10 - 20 min - 50/50
Col. Temp.	: UV 210 nm
Detection	: 0.2 mL/min
Sample	: 40 °C : Digested BSA 2 $\mu$ L

**MonoSpin Trypsin provide rapid and efficient protein digestion at room temperature in 10 mins.**

## List of References


Products	Target Analytes	Sample Matrix	Concentration	Recovery Rate	Detection	Reference No.
MonoSpin® C18	amitraz, metabolites	serum	5 ng/mL	95.5, 92.2 %	LC-MS	[1]
	dibucaine, naphazoline	serum	5 - 10 ng/mL	70.2 - 78.6 %	LC-MS	[2]
	MA, AP, MDA, MDMA	urine	100 ng/mL	96 - 111 %	LC-UV	[3]
	9 cold medicines	serum	5 - 50 ng/mL	2.5 - 73.8 %	GC-MS	[4]
	amphetamines (AP, MA, MDA, MDMA)	urine	5 - 10 ng/mL	84 - 94 %	GC-MS	[5]
	epersin	serum	0.5 ng/mL	92.8 - 96.0 %	GC-MS	[6]
	paraquat, diquat, fenitrothion	serum, urine	25 - 100 ng/mL	51.3 - 106.1 %	GC-MS	[7]
	arsenics	urine	1 ng/mL	91.9 - 106.5 %	GC-MS	[8]
	MAM-2201	blood	1 ng/mL	-	LC-MS/MS	[9]
	α-PVP, α-PBP	urine	1 ng/mL	82 - 100 %	GC-MS	[10]
	α-PVP, α-PBP	hair	0.2 ng/mL	75.5 - 101.5 %	LC-MS	[11]
	Phthalic acid esters	physiological saline	0.2 - 50 µg/L	71.2 - 107.3 %	-	[12]
	<desalting>	digested peptides	-	-	-	[13]
	<desalting>	iTRAQ labeled samples	-	-	-	[14]
	MAM-2201	blood	2.5 - 100 ng/mL	1 ng/mL	-	[15]
	Naringin	grapefruit juice	10 - 500 µM	10 µM	-	[16]
MonoSpin® SCX	opiates benzodiazepines, metabolites	urine serum	10 ng/mL 1 - 10 ng/mL	69.2 - 98.9 % 83.3 - 112.3 %	LC-MS	[17]
	<Pre-column fluorescence derivatization>	-	-	-	-	[18]
	<desalting of amino acid>	-	-	-	-	[19]
MonoSpin® C18-CX	acidic and basic drugs	urine	1 - 25 ng/mL	65 - 123 %	GC-MS	[20]
	<halogenated compounds>	cells	-	-	-	[21]
MonoSpin® C18-AX	amphetamines (AP, MA), opiates, THC	urine	2 - 10 ng/mL	93.1 - 108.1 %	GC-MS	[22]
MonoSpin® PBA	Adenosine	urine	6 µM	80 - 113 %	-	[23]

- [1] J. Chromatogr., B 867 (2008) 99-104.
- [2] J. Chromatogr., B 872 (2008) 186-190.
- [3] J. Chromatogr., A 1208 (2008) 71-75.
- [4] Chromatographia., 70 (2009) 519-526.
- [5] Anal. Chim. Acta., 661 (2010) 42-46.
- [6] J. Health Sci., 56 (2010) 598-605.
- [7] Anal. Bioanal. Chem., 400 (2011) 25-31.
- [8] J. Sep. Sci., 35 (2012) 2506-2513.
- [9] Forensic Toxicol., 31 (2013) 333-337.
- [10] Forensic Toxicol., 32 (2014) 68-74
- [11] J. Chromatogr., B 942-943 (2013) 15-20.
- [12] J Pharm Anal., 1 (2011) 92-99


- [13] Proteomics., 13 (2013) 751-755
- [14] Journal of proteomics., 84 (2013) 40-51
- [15] Forensic Toxicol., 31 (2013) 333-337
- [16] The Journal of Clinical Pharmacology., 54 (2013)
- [17] J. AOAC Int., 94 (2011) 765-774.
- [18] Biomed. Chromatogr., 26 (2012) 147-151.
- [19] Orig Life Evol Bjsoph., 43 (2013) 99-108
- [20] J. Sep. Sci., 34 (2011) 2232-2239.
- [21] Toxicology., 314 (2013) 22-29
- [22] Forensic Toxicol., 31 (2013) 312-321.
- [23] Biosensors and Bioelectronics., 41 (2013) 379-385

## Recovery of Metal Ions using MonoSpin ME

MonoSpin ME is bonded with iminodiacetic acid and optimal for the recovery and purification of metal ions. Specifically, it is excellent for the extraction and purification of trace Pb in blood or urine. Additionally, it is appropriate for removing inorganic divalent cations from sample to prevent ion suppression for LC-MS/MS applications.

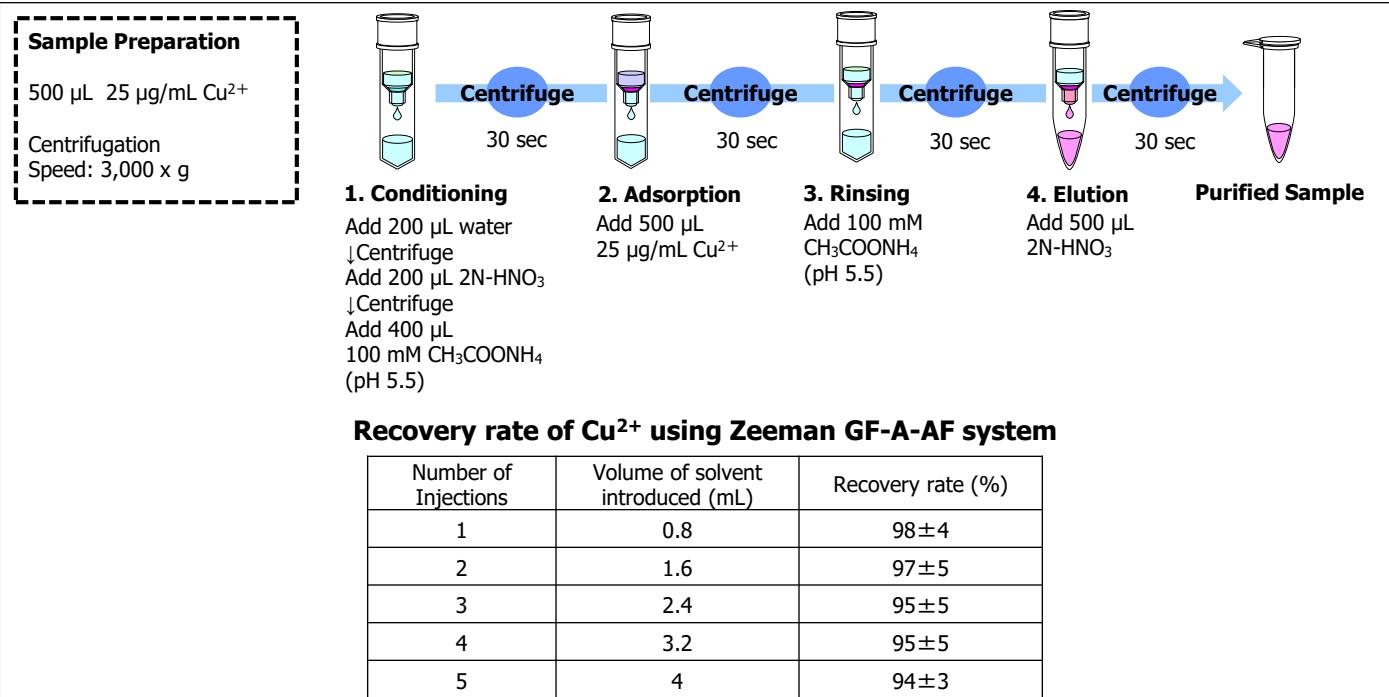


### Retention Characteristics of Metal Element using Iminodiacetic Acid Functional Groups with Various pH

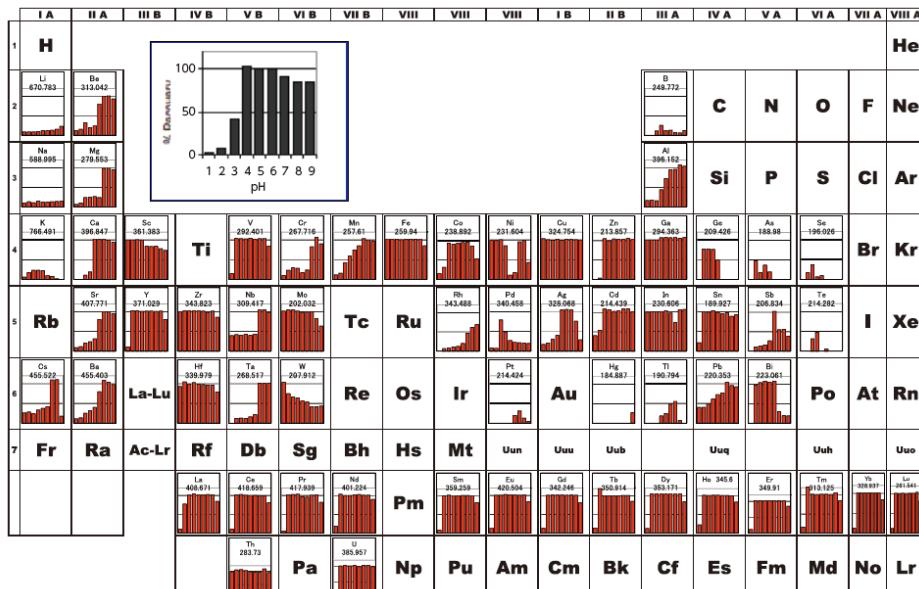

## Removal of Phospholipids using MonoSpin Phospholipid


MonoSpin Phospholipid removes more than 90% of phospholipids from biological samples resulting in eliminating ion suppression in LC-MS/MS analysis. The MonoSpin Phospholipid also removes phospholipids from a serum sample volume of 50  $\mu$ L.

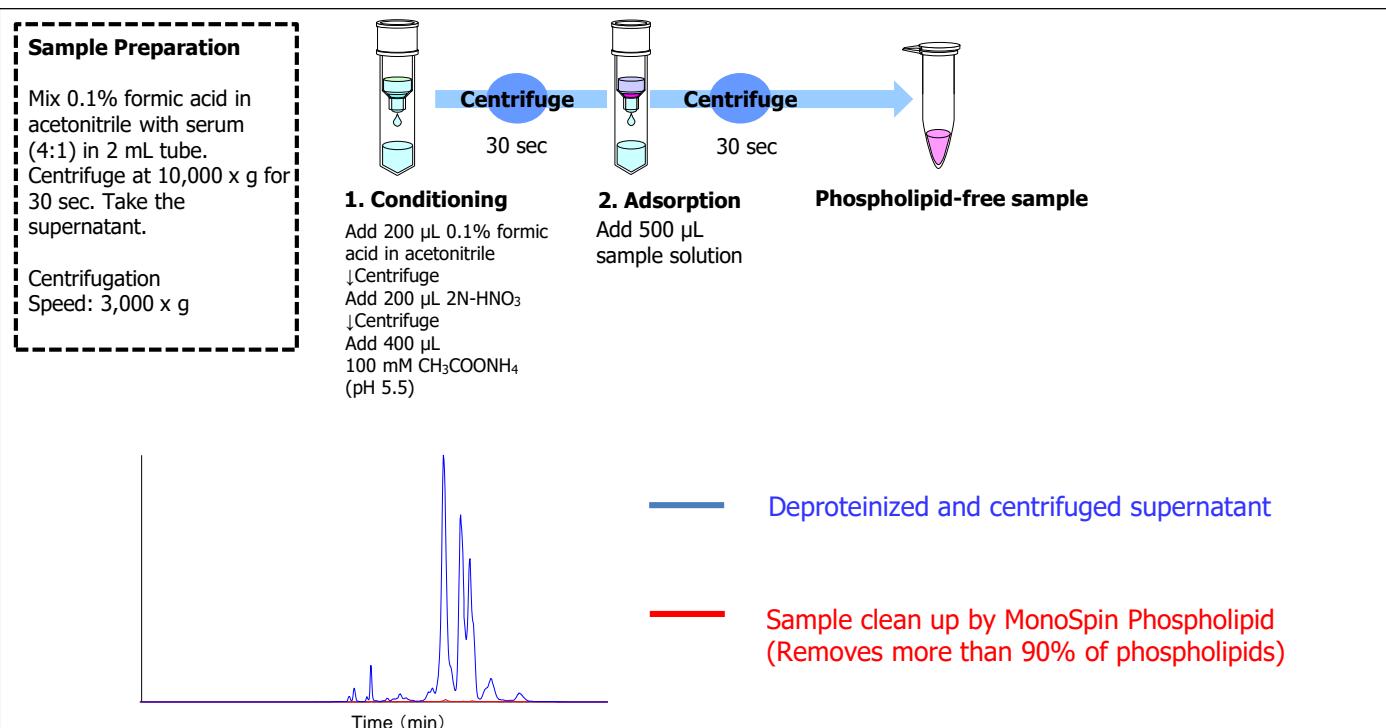

## Phospholipid Removal Efficiency of MonoSpin Phospholipid

### Retention Mechanism of Phospholipids

Monolith skeletal structure coated with TiO<sub>2</sub> and ZrO<sub>2</sub> selectively interacts with metal oxides and phosphorylated compounds, resulting in removing more than 90 % of phospholipids.

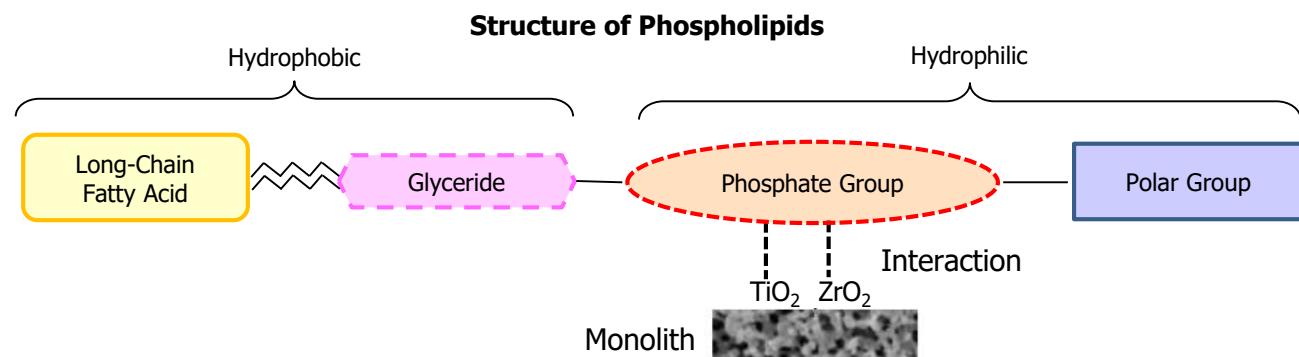


## Rapid Purification of Antibodies using MonoSpin ProA and ProG

MonoSpin ProA and MonoSpin ProG are immobilized with protein A or protein G onto a silica monolith offering rapid purification of antibodies. A 96-well plate format is also available for high throughput purification.

### Features

The silica is modified with a hydrophilic polymer and then immobilized with either Protein A or Protein G to prevent the adsorption of proteins, resulting in rapid purification and high recovery of antibodies.

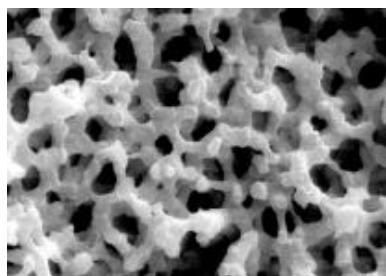


Specification	
Bonded Phase	Protein A or Protein G
Through-pore	2 µm
Meso-pore Size	60 nm
Disc Size	Φ4.6 x 1.5 mm
Sample Volume	50 - 500 µL
Recovery Rate	MonoSpin ProA:IgG 90 % (With 400 mg IgG) MonoSpin ProG:IgG 90 % (With 300 mg IgG)
Elution Volume	50 µL
Centrifugation speed	2,300 × g




**Antibody Compatibility Table**

Species	Antibody Class	Protein A	Protein G
Human	IgG	◎	◎
	IgG1	◎	◎
	IgG2	◎	◎
	IgG3	—	◎
	IgG4	◎	◎
	IgM	—	—
	IgA	—	—
	IgE	—	—
	IgD	—	—
	Fab	○	○
	ScFv	○	—

## Purification of IgG only in Five Minutes using MonoSpin ProA and ProG

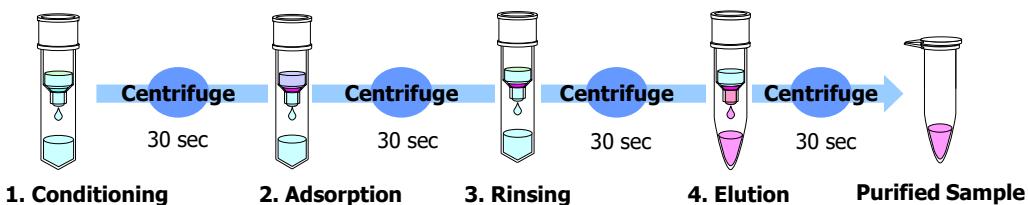

As shown below, the antibody concentrations were determined quantitatively from medium of CHO cells. The purified antibodies show very less impurities by the results from electrophoresis.

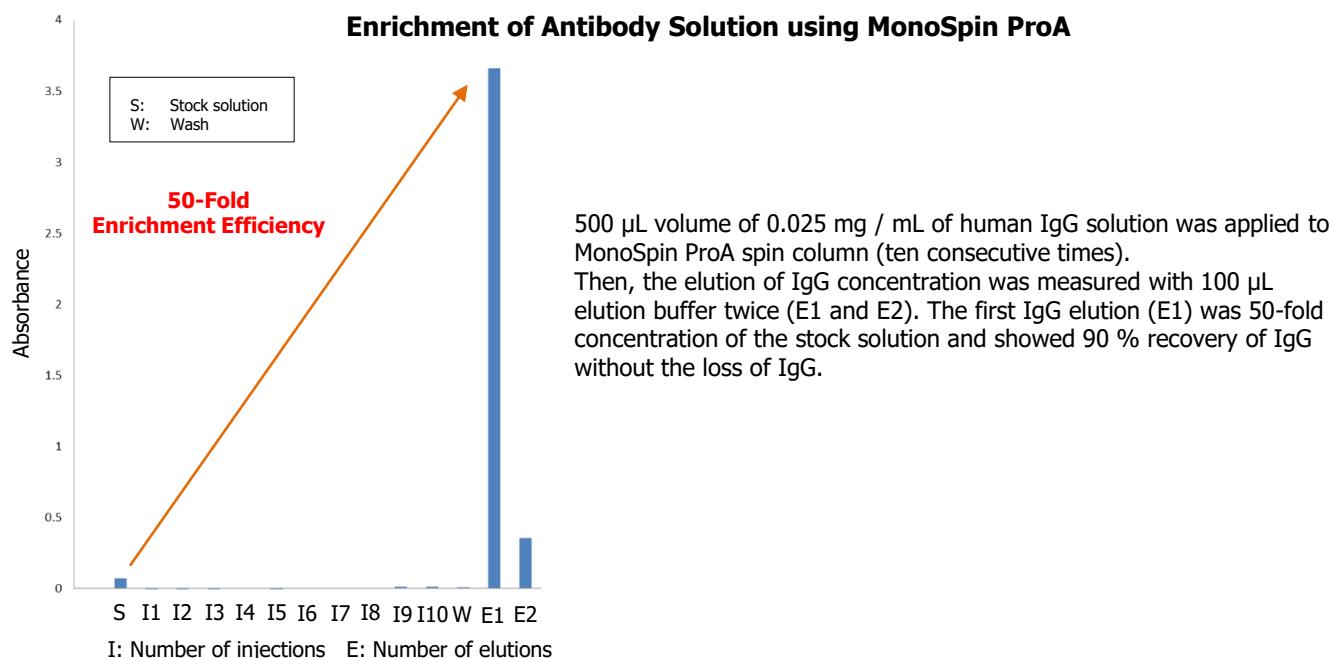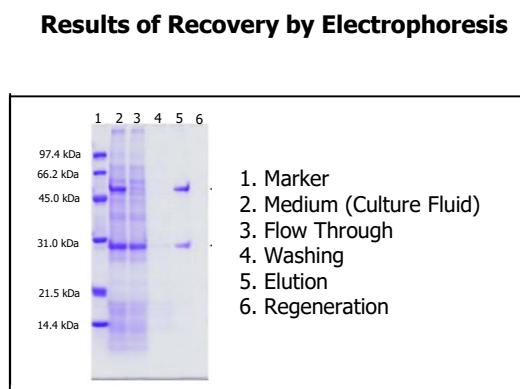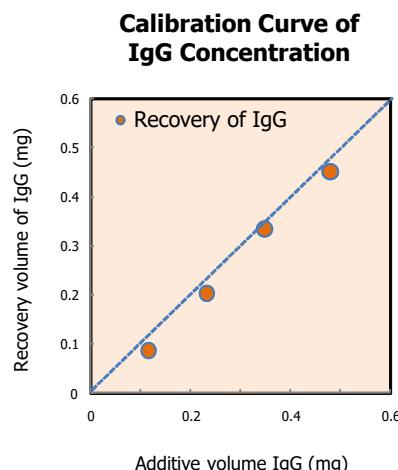


## Comparison of Elution Volume & Recovery Rate with other Brands' Products

MonoSpin ProA only requires 100  $\mu$ L elution buffer, providing a recovery rate of at least 90% IgG. On the other hand, other brands' products requires 400  $\mu$ L of elution buffer with a recovery rate of 70% IgG.


### MonoSpin ProA

90 % recovery rate of IgG with 100  $\mu$ L elution

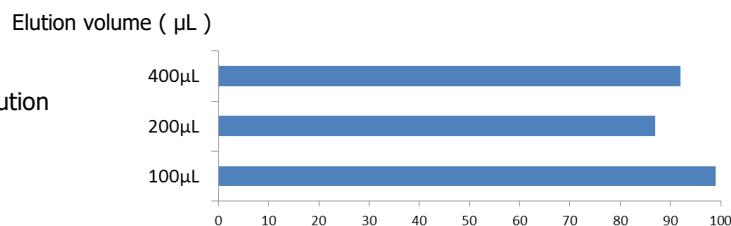


### Brand T's Product

60-65 % recovery rate of IgG with 400  $\mu$ L elution

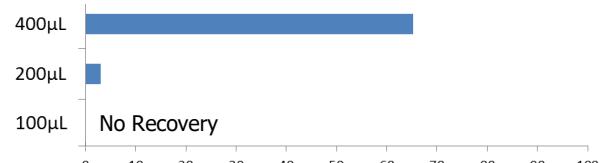


### Brand G's Product

65-70 % recovery rate of IgG with 400  $\mu$ L elution

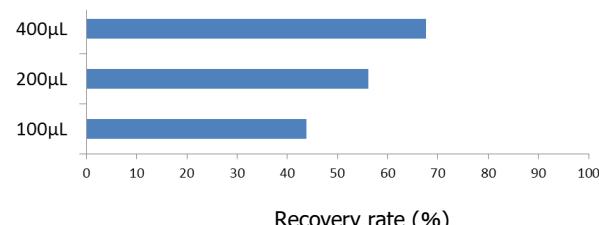

### Recovery Rate and Reproducibility of IgG from medium cultured CHO cells with MonoSpin ProA 96-Well Plate

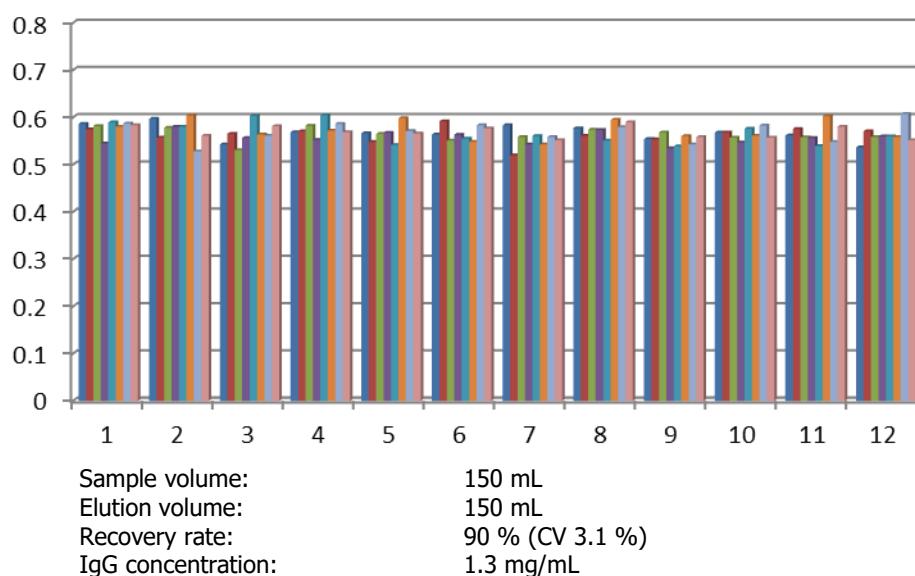

# MonoSpin Series

## Ordering Information

---

### MonoSpin S Type (Small) Columns

- Each MonoSpin S Type (Small) columns are attached with 1.7 mL recovery tubes and 2.0 mL waste tubes.

Description	Qty	Cat. No.
MonoSpin C18	50 pcs	5010-21700
	100 pcs	5010-21701
MonoSpin C18 FF	50 pcs	5010-21670
	100 pcs	5010-21671
MonoSpin Ph	50 pcs	5010-21733
	100 pcs	5010-21734
MonoSpin C18-AX	50 pcs	5010-21735
	100 pcs	5010-21736
MonoSpin C18-CX	50 pcs	5010-21731
	100 pcs	5010-21732
MonoSpin SAX	50 pcs	5010-21720
	100 pcs	5010-21721
MonoSpin SCX	50 pcs	5010-21725
	100 pcs	5010-21726
MonoSpin NH <sub>2</sub>	50 pcs	5010-21710
	100 pcs	5010-21711
MonoSpin CBA	50 pcs	5010-21729
	100 pcs	5010-21730
MonoSpin Amide	50 pcs	5010-21727
	100 pcs	5010-21728
MonoSpin PBA	50 pcs	5010-21715
	100 pcs	5010-21716
MonoSpin TiO	50 pcs	5010-21705
	100 pcs	5010-21706
+ MonoSpin Trypsin	50 pcs	7820-11300
	100 pcs	7820-11301
MonoSpin ME	50 pcs	5010-21737
	100 pcs	5010-21738
MonoSpin Phospholipid	50 pcs	5010-21698
	100 pcs	5010-21699

\* MonoSpin Trypsin must be refrigerated when not in use.



MonoSpin S Type (Small)



Recovery Tube  
(1.7 mL)



Waste Tube  
(2 mL)

## Ordering Information

---

### MonoSpin L Type (Large) Columns

Description	Qty	Cat. No.
MonoSpin L C18	30 pcs	7510-11320
MonoSpin L SAX	30 pcs	7510-11321
MonoSpin L SCX	30 pcs	7510-11322
MonoSpin L NH2	30 pcs	7510-11323
MonoSpin L CBA	30 pcs	7510-11324
MonoSpin L ME	30 pcs	7510-11325
MonoSpin L Phospholipid	30 pcs	7510-11326



MonoSpin L Type (Large)

\* Each MonoSpin L Type (Large) columns does not come with any recovery and waste tubes.

\* Please prepare a 50 mL centrifuge tube separately (Ex: Falcon tube).

### MonoSpin ProA, MonoSpin ProG

Description	Qty	Cat. No.
MonoSpin ProA	10 pcs	7510-11310
MonoSpin ProG	10 pcs	7510-11311
MonoSpin ProA 96-Well Plate	1/pk	7510-11312
MonoSpin ProG 96-Well Plate	1/pk	7510-11313

\* MonoSpin ProA, ProG must be refrigerated when not in use.

### MonoSpin S Type (Small) Trial Kits

- The following trial kits are available for purchase to test a whole range of MonoSpin columns to make the best decision on which MonoSpin to use.

Description	Available Phases	Qty	Cat. No.
MonoSpin Trial Kit 1	C18, TiO, SCX, SAX, 10 pcs each.	10 pcs/4 pk	5010-21740
MonoSpin Trial Kit 2	C18, Amide, CBA, NH2, 10 pcs each.	10 pcs/4 pk	5010-21741
MonoSpin Trial Kit 3	SCX, SAX, CBA, NH2, 10 pcs each.	10 pcs/4 pk	5010-21742

- MonoSpin Trial Kit 1: Optimal for drug extraction in biological samples & purification of pesticides.
- Monospin Trial Kit 2: Compatible with both hydrophilic/hydrophobic applications. Optimal for purification of peptide and sugar chains.
- MonoSpin Trial Kit 3: Optimal for purification of ionic analytes.

## FastRemover for Protein

### Maximizes Sample Yield

FastRemover is a 96-well type filter plate ideal for preparing precipitated protein samples. High-throughput processing of plasma samples is performed simply, accurately, and reproducibly.

### Features

- Easy filtration of biological samples.
- Trace analytes can be processed with minimal sample loss owing to the low volume design of the elution tip and filter.
- Perfect for processing with automated vacuum instruments.
- High sensitivity analysis is unaffected by contamination from plasticizers or other impurities found in other 96-well plates.
- Removal of microparticle contaminants enables injection to LC/MS/MS directly from the collection plate.


### Typical Protocol using FastRemover for Protein

To demonstrate the performance of FastRemover for Protein, a BSA solution was prepared as follows:

#### Performance of Removal of Proteins


1. 200 uL of plasma is thoroughly mixed in a test tube containing 800uL of acetonitrile.
2. The FastRemover and collection plate are attached to a vacuum manifold.
3. The BSA sample mixture is loaded into the 96-well plate and vacuum applied above 0.02 Mpa (0.2 Bar) for 2 minutes.

\* Methanol can be used as well as a replacement of acetonitrile.

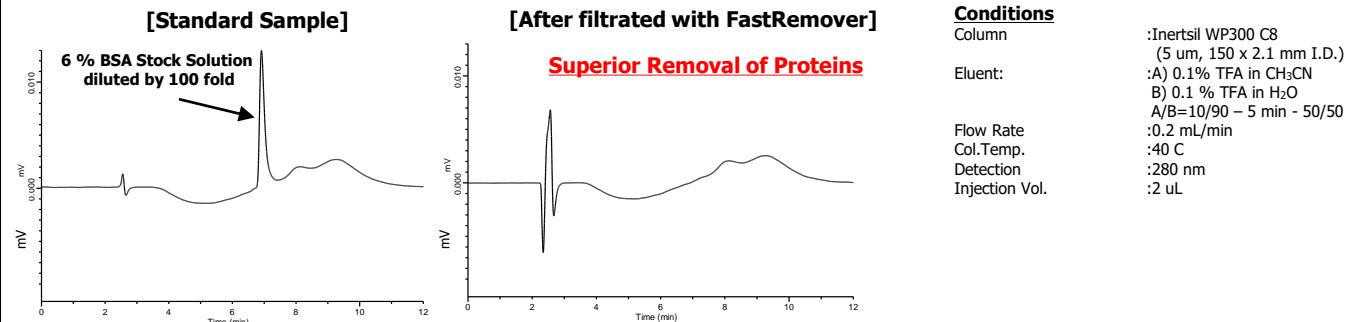

## Adsorption Test

A standard mixture containing 7 compounds were analyzed to evaluate potential non-specific adsorption to the plate. As shown in the following chromatograms, FastRemover for Protein provides minimal loss of target samples.

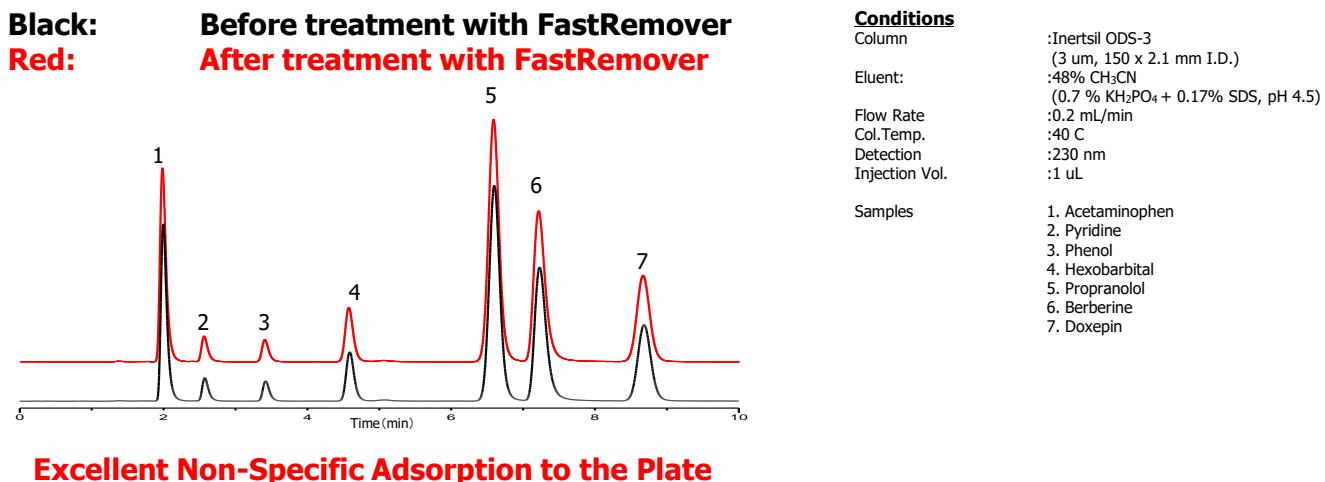

## Ordering Information

### FastRemover for Protein

Description	Qty	Cat. No.
FastRemover for Protein (0.45 $\mu$ m) 96-well	1/pk	7820-11001
	5/pk	7820-11005
FastRemover for Protein (0.20 $\mu$ m) 96-well	1/pk	7820-11011
	5/pk	7820-11015

### Related Accessories

Description	Qty	Cat. No.
Vacuum Manifold with shims	1 Set	5010-33101
Sealing Mat for Microplate, WSM-3SX (PTFE/SILCON)	5/pk	1030-43831
Sealing Tape for Microplate, (Polyolefin)	100/pk	1065-70002

## FastRemover for Phospholipid

### Rapid and Efficient Removal of Proteins and Phospholipids

The FastRemover for Phospholipid 96-well plate deliver a rapid and effective removal of proteins and phospholipids in plasma and serum samples without sacrificing the recovery of your target analytes.

### Features

- Simple & easy protocol to remove proteins and phospholipids.
- High sensitivity analysis is unaffected by contamination from plasticizers or other impurities found in other 96-well plates.
- Removal of microparticle contaminants enables injection to LC/MS/MS directly from the collection plate.
- Removes more than 90% of phospholipids resulting in eliminating ion-suppression.
- Prolong HPLC/UHPLC column lifetime by removing proteins and phospholipids that can damage your column.

### Typical Protocol using FastRemover for Phospholipid

The presence of phospholipids in plasma or serum samples is one of the major problems in LC/MS-(MS) analysis. Phospholipids can build up on your MS system and bleed off the HPLC/UHPLC column, causing ion suppression, shifts in retention time and peak shape and necessitating time consuming column and system maintenance. Use of FastRemover for Phospholipid 96-well plate will eliminate these effects and extend the lifetime of your HPLC/UHPLC column and deliver more predictable/accurate mass spectrometry results.

#### Easy Protocol by FastRemover for Phospholipid

##### Step 1: Solvent Loading

Add 400  $\mu$ L of 1% Formic Acid in Acetonitrile into the wells

##### Step 2: Sample Loading

Add 100  $\mu$ L of serum sample into the wells

##### Step 3: Mixing

Aspirate the samples up & down couple of times by a manual pipette or an automated pipetting system may be used to ensure complete mixing

##### Step 4: Analysis


Collect the extracted sample from the 96-well plate & inject to LC/MS/MS

\* Traditional Protein Precipitation method:

Adding acetonitrile to sample and collecting the supernatant layer

RED: FastRemover for Phospholipid

BLUE: \* Traditional Protein Precipitation

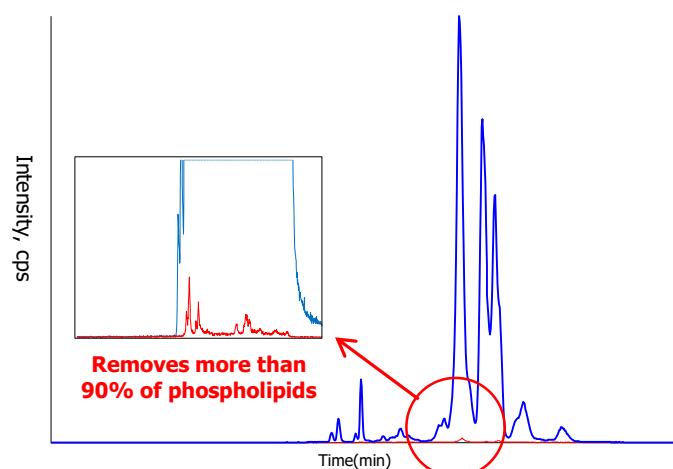


#### Comparison of Phospholipid Removal between

\* Traditional Protein Precipitation method and  
FastRemover for Phospholipid


## Extend HPLC/UHPLC Column Lifetime

Over the course of multiple injections, phospholipids build up and can lead to reduced column lifetime, showing increase in column back pressure, decrease in column sensitivity and efficiency. The figure on the right illustrates the removal efficiency of phospholipids, proteins and microparticles by FastRemover for Phospholipid.

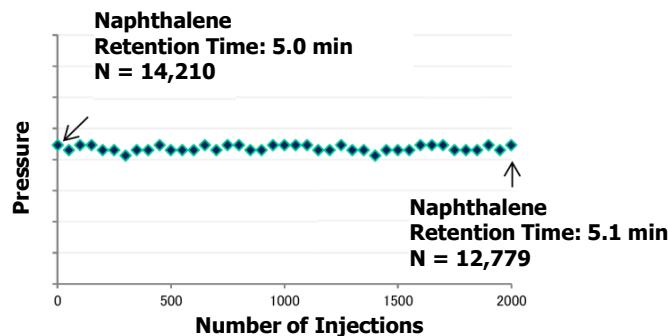


## Industry Leading High Recovery for Bioanalysis

As shown below, the FastRemover for Phospholipid 96-well plate deliver a rapid and effective removal of proteins and phospholipids in plasma and serum samples without sacrificing the recovery of your target analytes.

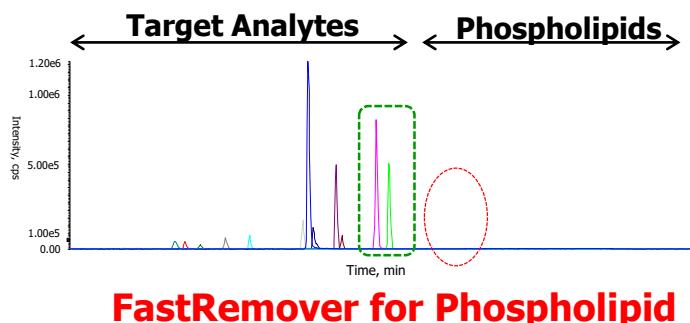

As shown on the left, not only FastRemover for Phospholipid completely removes phospholipids, but also provide high recovery even for those highly hydrophobic analytes.

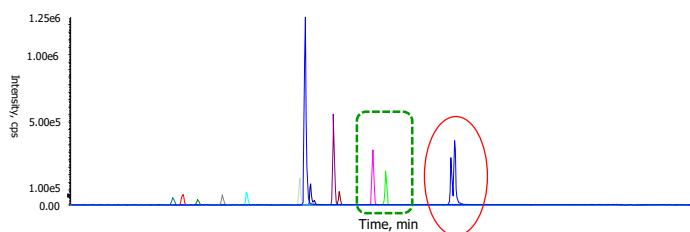


Brand A show adsorption of hydrophobic analytes resulting in poor recovery and elution of phospholipids.

Brand A Phospholipid Removal Plate


## Comparison of Recovery Rate using Various Solvents for Deproteinization

The following seven solvents were used to deproteinate a serum sample. As a result, 0.1% formic acid in 100% acetonitrile showed the best recovery for not only basic, but also for acidic compounds.


1. Acetaminophen




2. Scopolamine




3. Theophylline




4. Caffeine




5. Metoprolol

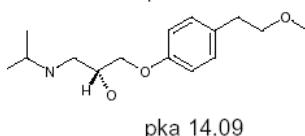


6. Propranolol




7. Diphenhydramine




8. Doxepin




9. Imipramine




10. Warfarin




11. Amitriptyline



12. Ketoprofen



13. Diclofenac



The  
Best  
Results

Analyte	CH <sub>3</sub> OH	CH <sub>3</sub> CN	0.1%HCOOH -CH <sub>3</sub> OH	0.1%HCOOH -CH <sub>3</sub> CN	1%HCOOH -CH <sub>3</sub> CN	0.1%HCOONH <sub>4</sub> -CH <sub>3</sub> OH	1%HCOONH <sub>4</sub> -CH <sub>3</sub> OH
1.Acetaminophen	116.2	92.3	106.9	103.5	102.2	2.7	92.2
2.Scopolamine	75.2	87.4	86.0	87.8	83.6	0.9	68.9
3.Theophylline	104.2	95.7	107.2	96.3	94.1	5.1	94.9
4.Caffeine	97.1	98.2	106.4	97.7	90.6	6.0	98.3
5.Metoprolol	90.7	98.4	89.3	90.8	95.5	1.0	76.8
6.Propranolol	88.2	97.4	92.6	106.4	102.9	1.5	78.3
7.Diphenhydramine	89.1	106.6	92.8	106.3	102.5	2.7	75.7
8.Doxepin	76.9	101.6	86.1	107.2	97.7	1.0	64.7
9.Imipraine	80.9	105.8	82.1	99.9	99.7	1.0	72.8
10.Warfarin	85.4	98.6	84.5	103.1	108.4	1.1	80.6
11.Amitriptyline	60.6	103.9	54.8	86.9	90.9	0.9	73.2
12.Ketoprofen	N.D.	39.3	1.4	98.1	108.6	1.9	39.2
13.Diclofenac	8.4	89.2	4.4	102.9	104.9	1.1	67.9

## Ordering Information

---

### FastRemover for Phospholipid

Description	Qty	Cat. No.
FastRemover for Phospholipid (0.2 µm)	1 pcs	7510-11021



## EVSecond

### Exosome Purification Columns

Recent studies have reported significant roles of extracellular vesicle "Exosome" in development and progression of various diseases including cancer metastasis. Therefore exosomes are considered as attractive targets for biomarkers and drug development. However, it remains difficult to isolate high-purity exosomes from biological fluids such as serum. EVSecond is a size exclusion chromatography open column optimized for effective purification of exosomes. Highly-purified exosomes can be easily collected from serum, plasma, or cell culture supernatant.

### Features

- Simple gravity-flow handling without ultracentrifugation.
- EVSecond-purified exosomes possess efficient purity for comprehensive miRNA, proteome, and metabolome analysis.
- Exosomes are gently eluted in PBS without structural damage, allowing re-administration experiments of collected exosomes to cells or animals.

### Advantages Over Traditional Procedures

- Much higher-purity exosomes can be obtained compared to ultracentrifugation or polymer precipitation methods.
- Unlike immuno-affinity purification using anti-tetraspanin antibodies, whole exosomes can be collected regardless of surface antigen profiles.

### Typical Protocol using EVSecond

Gravity-flow is applied to each step.

1. Set columns on GL-SPE EXO fraction rack after mixing beads gently and thoroughly.



2. Block beads with 0.22 µm filter-purified FBS.



3. Equilibrate columns with PBS.




4. Load 50-700 µL 0.22 µm filter-purified samples (serum, plasma, or cell culture supernatant).



5. Load PBS and collect appropriate fractions including exosomes.

#### GL-SPE EXO Fraction Rack

Open column rack optimized for EVSecond. It helps smooth column handling and fractionation.

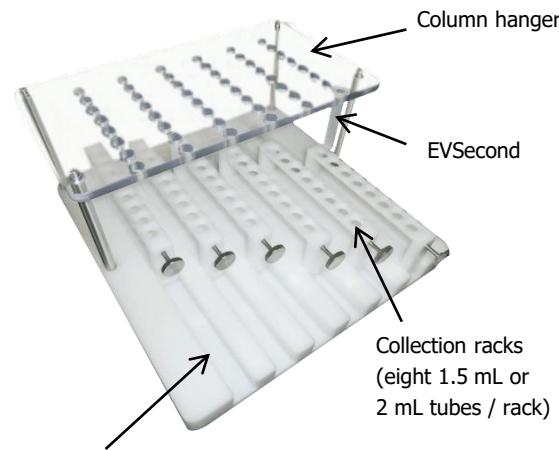


Dimensions: 300(W) x 300(D) x 150(H) mm

\* Exosome-containing fractions can be identified by western blotting or ELISA experiments detecting tetraspanins (CD9, CD63, CD81, etc.)

## Purification of Exosomes from Human Serum

A large amount of free proteins, metabolites, and nucleotides are involved in serum samples. Insufficient purification of exosomes often causes co-detection of non-exosomal components, leading to incorrect quantification results in omics studies. Exosomes were isolated from 100, 200, 300, or 700  $\mu$ L of human serum using EVSecond method. Exosomes were clearly separated from serum free proteins such as albumin or immunoglobulins.

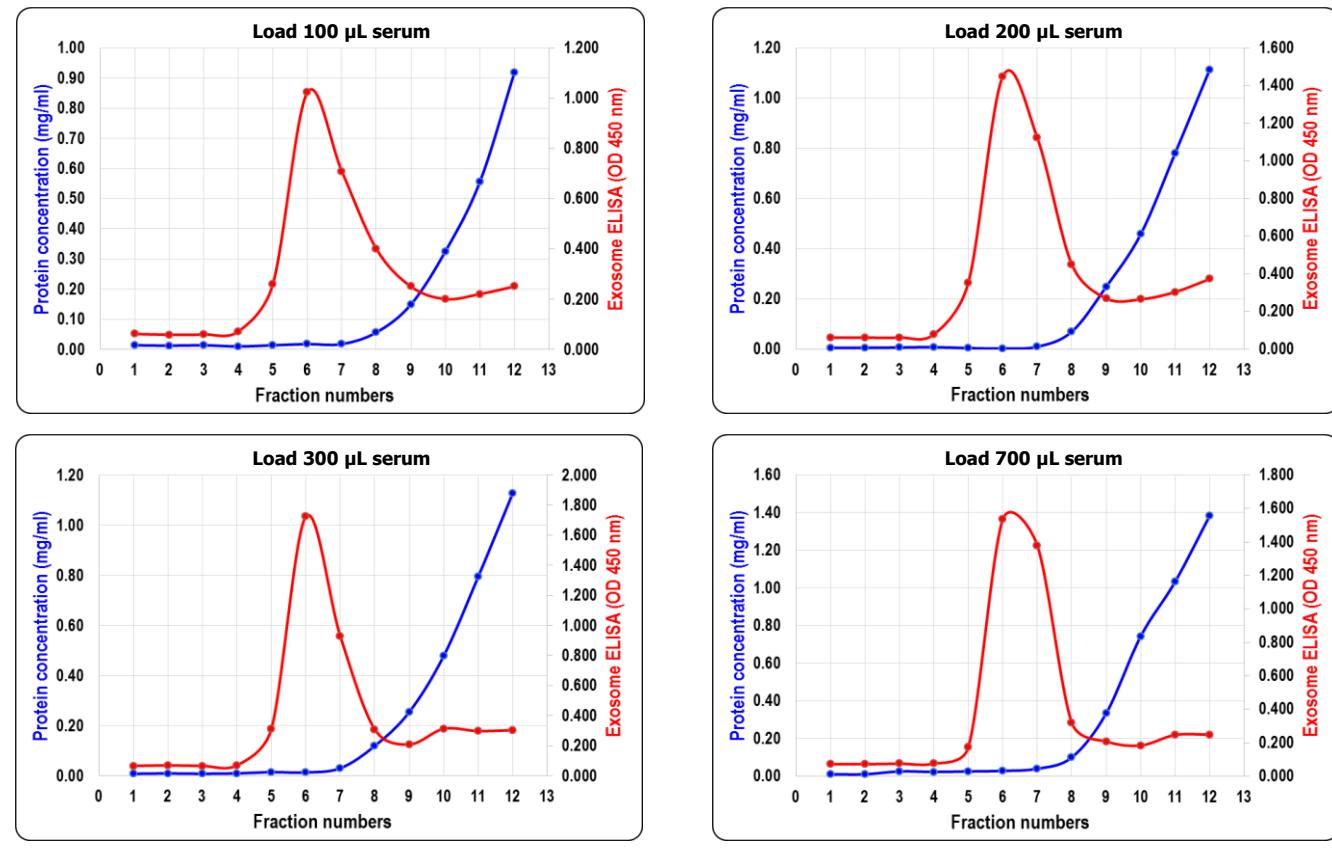

Data provided by Dr. Koji Ueda from Graduate School of Frontier Sciences, The University of Tokyo

## Ordering Information

### EVSecond

Description	Qty	Cat. No.
EVSecond	10 pcs	5010-21390
	25 pcs	5010-21392
GL-SPE EXO Fraction Rack	1 set	5010-50450

EVSecond was developed based on the cooperation from Dr. Koji Ueda from Graduate School of Frontier Sciences, The University of Tokyo.

## MonoFas DNA Purification Kit I



### DNA Extraction & Purification

MonoFas DNA Purification Kit I purifies DNA from PCR products and agarose gels. Purified DNA can be used for sequencing, cloning/ligation, restriction digests, etc.


### Features

- Multiple Roles – Purifies DNA from PCR matrices or agarose gels.
- Rapid purification in about 4 minutes.
- High recovery rates even from sample volumes as low as 10  $\mu$ L.
- Purify DNA fragments from 35 bp to 35 kbp.


#### High Recovery from Trace Volume Samples

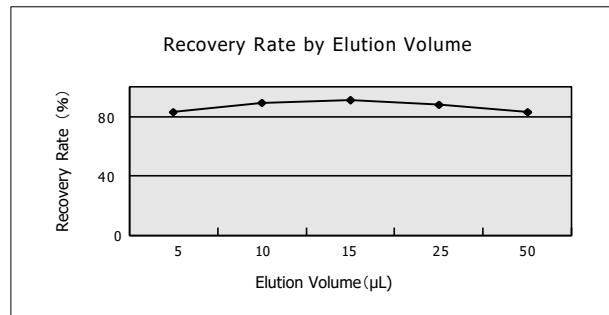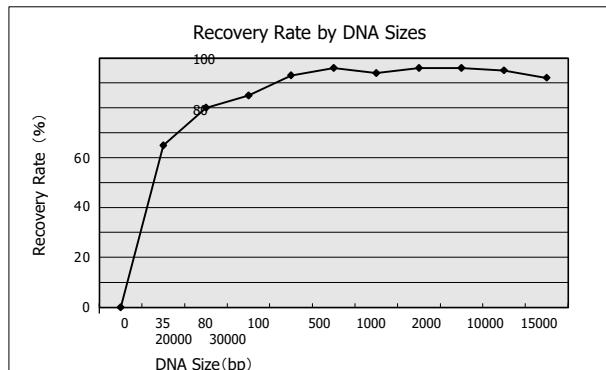

#### Purify DNA fragments from 35bp up to 35kbp

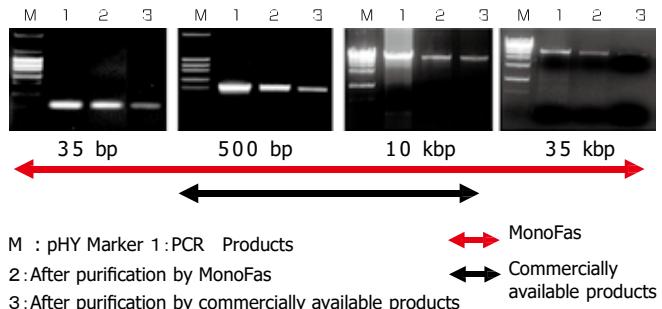

#### Large Quantities of Agarose Gels can be Processed



MonoFas routinely extracts DNA from up to 1 g of agarose gel at once.

400 bp  
M : pHY Marker  
1 : Unpurified PCR products 2 :  
Purified from agarose gel  
(MonoFas DNA Purification Kit I )

## Specifications

Description	Purification from PCR products	Extraction from agarose gel
Time	4 mins	9 mins
Maximum DNA Binding Amount	<10 µg	<10 µg
Maximum Agarose Gel Throughput	—	<1g
Minimum Elution Amount	10 µL	10 µL
Column Volume	1 mL	1 mL
Processable DNA Range	35 bp - 35 kbp	35 bp - 35 kbp
Recovery Rate	>85 % (100 bp - 5 kbp) >60 % (5 kbp - 35 kbp)	>80 % (100 bp - 5 kbp) >50 % (5 kbp - 35 kbp)
Primer Removal Percentage	95 %	—


## Typical Protocol using MonoFas DNA Purification Kit I

### 1. Purification of PCR products

Load the PCR products and Buffer A (10 times the volume of PCR products) into the spin column.


### 2. Extraction from agarose gel

Add the Buffer A (same volume as the agarose gel), dissolve for 5 mins at 60 °C then load it into the spin column.

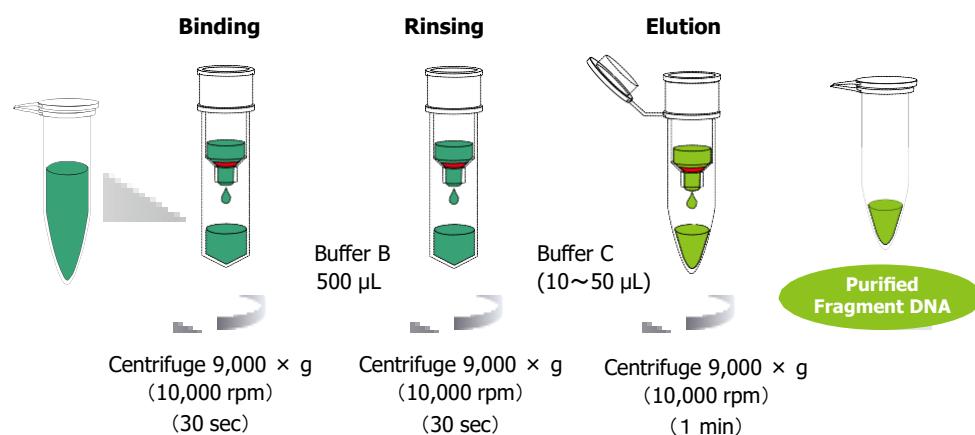

## Accurate Sequence Analysis

Greater than 98 % precision by fluorescent sequence method and more than 500 bases can be analyzed.

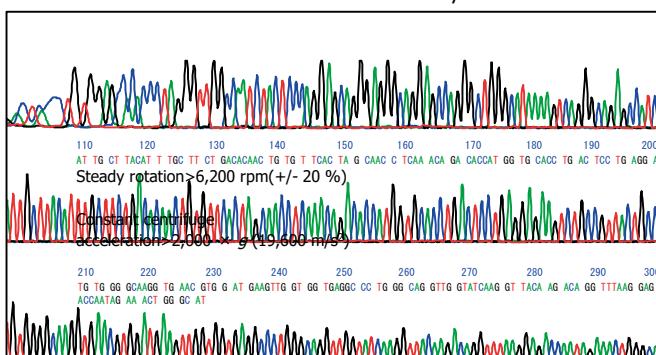

Condition: Cycle sequencing method with Big Dye Terminator v3.1 manufactured by ABI  
Model: ABI 3730 Genetic Analyzer

## Easy Centrifuge Operation



2 mins : DNA purification from PCR products  
7 mins : DNA purification from agarose gel

## Ordering Information

---

### MonoFas DNA Purification Kit I

Description	Qty	Cat. No.
MonoFas DNA Purification Kit1, EXPORT	50 pcs	5010-21530
	100 pcs	5010-21531
	250 pcs	5010-21532



# MonoFas DNA Purification Kit III


## Plasmid DNA Extraction from E.coli

MonoFas Plasmid Extraction Kit III is designed to purify plasmid DNA from E. Coli cultures. The extracted plasmid DNA can be used without further purification for sequence analysis, restriction digestion, cloning/ligation, etc.

## Features


- Rapid Plasma Purification in 8 minutes.
- Highly Purified Plasmid DNA.
- Wide Variety of Functional Groups
- BAC Clone Purification can also be performed.
- Stable Recovery Rate

### Extraction of Highly Purified 2.6 kbp Plasmid DNA from 1.5 mL E. Coli (DH5a)

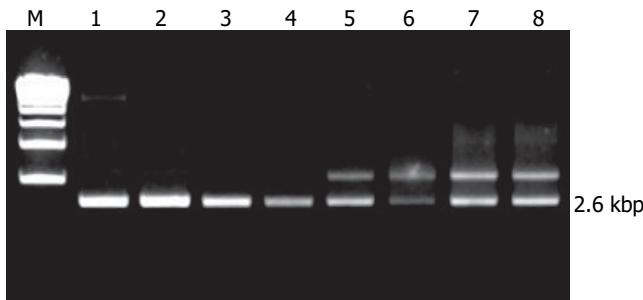

M: DNA Marker  
1~4: MonoFas 5, 6: Brand A 7, 8: Brand B

### Highly Reproducible Extraction of Low-Copy 2.6 kbp Plasmid from E. Coli (JM109)

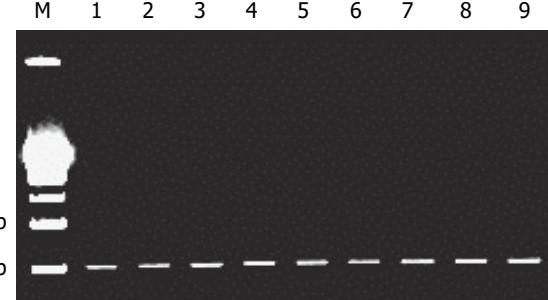

M: pHY Marker  
1~9: MonoFas (Low-Copy 2.6 kbp Plasmid)

## Ordering Information

### MonoFas DNA Purification Kit III

Description	Qty	Cat. No.
MonoFas DNA Purification Kit3, EXPORT	50 pcs	5010-21533
	100 pcs	5010-21534
	250 pcs	5010-21535

## Other MonoFas Series

### **MonoFas BAC Extraction Kit V**

**Efficient Isolation of BAC, Cosmid DNA**

---

### **MonoFas Cultured Cell DNA Extraction Kit VI**

**Isolation of High Yields of Pure DNA in 5 mins without Desalting & Damaging DNA**

---

### **MonoFas DNA Bacteria Extraction Kit VII**

**DNA Extraction from Gram Positive & Negative Bacteria**

---

### **MonoFas DNA Buccal Swabs Extraction Kit VIII**

**DNA Extraction from Buccal Swabs without Desalting**

---

### **MonoFas DNA Mouse and Rat Tail Extraction Kit IX**

**Rapid Extraction of DNA from Mouse & Rat Tails**

---

### **MonoFas DNA Stool Extraction Kit X**

**Stool Extraction Kit Designed to Extract Bacteria & Epithelial Tissues in Intestine**

---

### **MonoFas DNA Processed Food Extraction Kit XI**

**Rapid Extraction of DNA from Processed Food**

---

### **MonoFas Plant DNA Extraction Kit XII**

**Rapid Extraction of DNA from Processed Food**

---

For products details, please inquire.

## InertSearch Application Notes

Access to the latest pharmaceutical, life science, environmental and food applications at

[www.giscescences.com/tech/inertsearch](http://www.giscescences.com/tech/inertsearch)



# Worldwide Ordering Information

## **GL Sciences, Inc. USA**

4733 Torrance Blvd. Suite 255  
Torrance, CA 90503  
Phone: 310-265-4424  
Fax: 310-265-4425  
Email: [info@glsciencesinc.com](mailto:info@glsciencesinc.com)  
Web: [www.glsciencesinc.com](http://www.glsciencesinc.com)

## **GL Sciences B.V.**

De Sleutel 9  
5652 AS Eindhoven  
The Netherlands  
Phone: +31 (0)40 254 95 31  
Email: [info@glsciences.eu](mailto:info@glsciences.eu)  
Web: [www.glsciences.eu](http://www.glsciences.eu)

## **International Distributors**

Visit our Website at  
[www.glsciences.com/distributors](http://www.glsciences.com/distributors)

## **GL Sciences, Inc. Japan**

22-1 Nishishinjuku 6-Chome  
Shinjuku-ku, Tokyo,  
163-1130, Japan  
Phone: +81-3-5323-6620  
Fax: +81-3-5323-6621  
Email: [world@gls.co.jp](mailto:world@gls.co.jp)  
Web: [www.glsciences.com](http://www.glsciences.com)

The specification are subject to change without notice due to continual improvements.

